



CAD-CAM  
solutions





## DYNAMIC ABUTMENT® SOLUTIONS

AV. BLONDEL, 54 3º · 25002 · LLEIDA (SPAIN)  
TEL. +34 973 289 580  
das@dynamicabutment.com  
www.dynamicabutment.com

The information included in this catalogue is exclusively addressed to professionals in dental sector.

All commercial trademarks mentioned herein are fully registered by their respective companies, and the images that appear are just to provide an orientation.

Talladium reserves the right to modify this document without previous notice.

Talladium is not responsible for the inadequate execution of these products if the warning indications corresponding to every reference are not contemplated.

All of the products listed in this brochure are marking in accordance with CE legislation. Some of the products are not authorized for sale and distribution or do not have a sales license in some countries according to other legislations (FDA, CMDCAS, etc.) Please ask for information: das@dynamicabutment.com

 Marking in accordance with CE legislation and applicable sanitary regulations



Visit our Online Store to find all our products and compatibilities :

[www.dynamicabutmentstore.com](http://www.dynamicabutmentstore.com)

4	DYNAMIC ABUTMENT® SOLUTIONS
5	RESEARCH & DEVELOPMENT
6	QUALITY CENTER
7	INTERNATIONAL CUSTOMER SERVICE
8	DYNAMIC SYSTEM
10	DYNAMIC SYSTEM FOR MILLING STRUCTURES
12	CAD/CAM WORKFLOW - DAS PRODUCTS
14	DYNAMIC μSCANBODY/ ADAPTOR
16	LAB SCANBODY
18	DYNAMIC TIBASE®/DYNAMIC 3TIBASE®
20	DYNAMIC TIBASE® GINGIVAL OPTIONS
22	DYNAMIC PREMILL3D®/ADAPTORS
24	DYNAMIC MILLING TOOL - DMTONE®
26	IDIGITAL ANALOG
28	DAS LIBRARIES
30	DAS CUSTOMIZED SERVICES
32	CAD-CAM
36	DYNAMIC SYSTEM - LIST OF COMPATIBILITES
52	DYNAMIC SYSTEM COMPATIBILITES
154	DYNAMIC SCREWS TECHNICAL SPECIFICATIONS
157	DYNAMIC SCREWDRIVER & DYNAMIC SCREWS
158	STRAIGHT SCREWS TECHNICAL SPECIFICATIONS
159	SCREWDRIVERS & STRAIGHT SCREWS
162	INTRAORAL SYSTEM COLORS ACCORDING TO COMPATIBILITY
166	DYNAMIC MILLING TOOL SPECIFICATIONS
168	SCREWDRIVER ADAPTOR/COMPLEMENTS
169	IDENTIFICATION PRODUCT/ SECURITY & TRACEABILITY
170	TALLADIUM GUARANTEE

## DYNAMIC ABUTMENT® SOLUTIONS

# 「THE **ART** OF CHANGE」

The dental sector has evolved more in recent years than in the last four decades. The arrival of digitalisation now reverberates through all laboratory and dental clinic work processes. This process brings with it new workflows and new tools to be used in the process.

The premise of “adapt or die” is a reality. And that is why research and innovation has enabled us to be at the forefront of sector digitalisation and first to provide our clients and associates with innovative technological solutions.

Since our founding over 15 years ago, we have been a revolutionary force in the dental sector, rejigging preconceived ideas of workflows, angled solutions and dental aesthetics. This is the art of change. Of doing something before anyone else. Of being dynamic.

The dental sector will continue to evolve and new work processes will arise. And, of course, Dynamic Abutment® Solutions will be at the cutting edge and the first to offer comprehensive solutions to these changes. This is the art of innovation, of revolution. This is **the art of CHANGE.**

## RESEARCH & DEVELOPMENT

「Focus on excellence and R&D&I has seen us become No.1 in angled solutions」

The R&D&I Department at Dynamic Abutment® Solutions is endorsed by the UNE 166002 certificate for R&D&I systems management.

It is actively involved in international projects, working alongside the main operators in the sector, contributing know-how in both production and machining and the design of digital hardware for CAD and production management (CAM).

Consequent to this work with the leading figures and companies in the sector, we develop new products that are rolled out from our own Production Center. The Production Center features next-gen equipment, enabling us to make prototypes prior to receiving the final thumbs-up for the product from the R&D&I Department.

The R&D&I Center ensures comprehensive control over all the development stages for new projects, allowing them to be transformed into new products featuring the top-notch safety and quality levels that characterise our output and reaching our clients as soon as possible.



## QUALITY CENTER

「 "Controlling our quality process ensures the safety of our products" 」

Dynamic Abutment® Solutions has a Quality Center with the very latest metrology and control, prototyping and physical-chemical treatment equipment, and sanitary areas for refitting and packaging health products in an ISO-8 clean room.

Controlling the whole quality process ensures that our products are measured, inspected and checked using the most advanced control methods in the sector. We guarantee the quality of our products from production all the way through to packaging.

Being present in international markets means we have the mandatory health certificates that cover our product:

CE marking, CMD/CAS regulations, or FDA certificates, among others.

Our primary concern from the very beginning has been the quality and safety of our products: UNE-EN ISO 9001:2015, UNE-EN ISO 13485:2016, and UNE 166002:2014.



## INTERNACIONAL CUSTOMER CENTER

「 "Our experience and know-how serving our clients and distributors" 」

The main objective of the exclusive Dynamic Abutment® Solutions Customer Service Center is to maintain a constant channel of communication with our distributors and associates.

Our products are available in over 45 countries across five continents, with guaranteed health product management and certificates for international markets.



We offer our clients technical support, along with immediate answers and solutions with direct support from the R&D&I technical department for even the most complex of cases.



We participate in fairs, events, conferences and training sessions through our distributors and associates.



Direct contact with and suggestions from our clients allows us to continue improving the quality of the products and services we offer.



# DYNAMIC SYSTEM

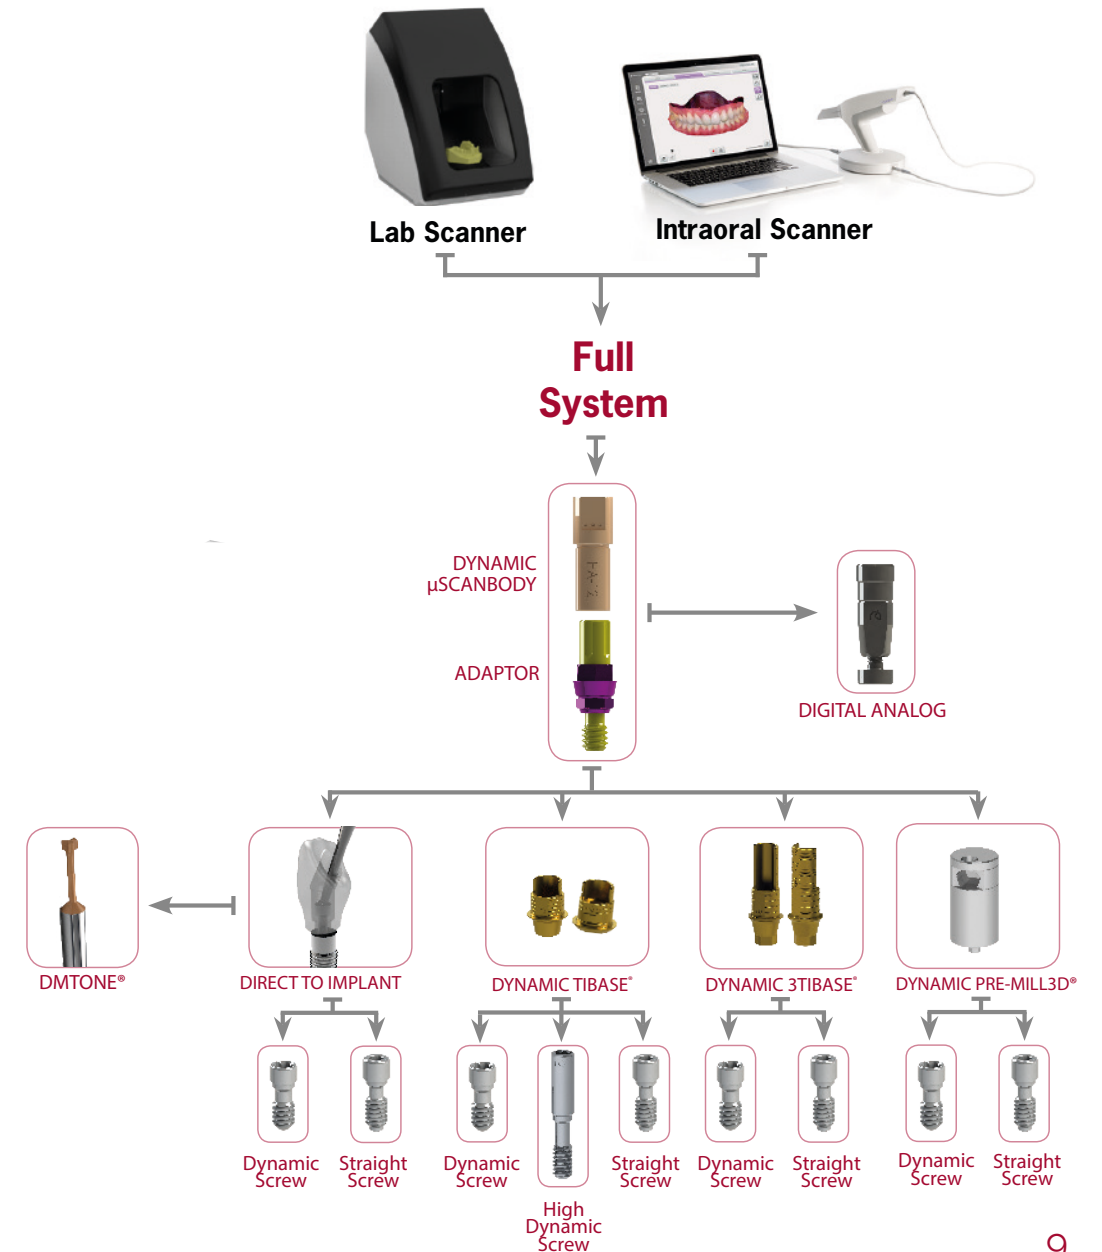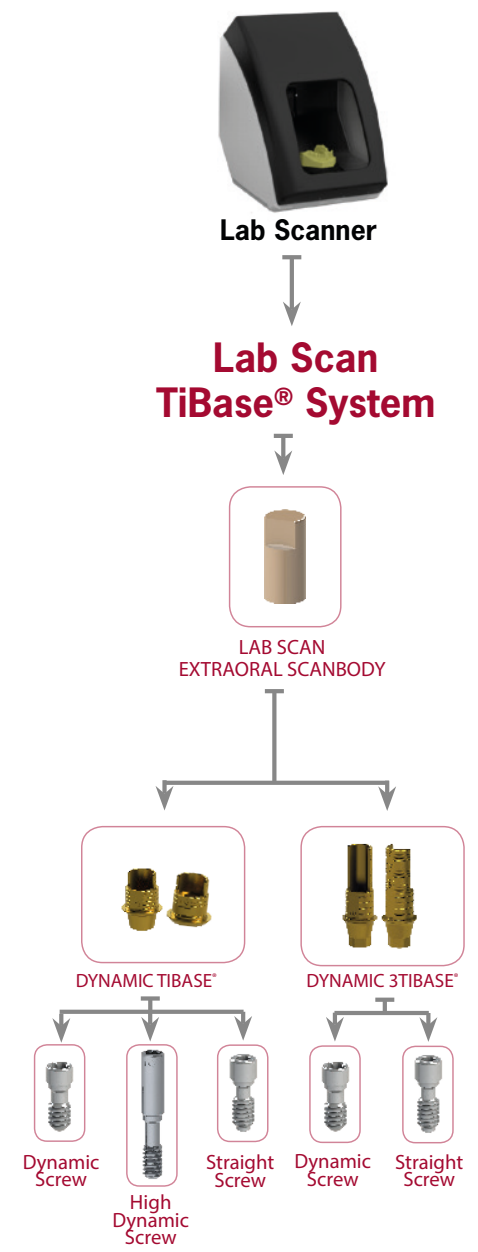

# DYNAMIC SYSTEM for MILLING STRUCTURES

The Screwdriver set of 3.0 Dynamic Abutment® System is used in those cases in which rectification of the entry of the screw due to an unfavorable position of the implants is necessary, improving the functionality and aesthetics of the milled prosthesis.

More than 500.000 cases resolved with **DYNAMIC SYSTEM**



PATENT NUMBER  
Dynamic Screwdriver  
EP 3 260 079

## Dynamic Screwdriver

Screwdriver with hexalobular head, exclusively to the 3.0 Dynamic Abutment® system.

Lengths: 18, 24, 32mm.



Our screwdriver has a contra-angle connection to make it easier to use with a dynamometer or manual ratchet, with the corresponding adaptors or handles.

## Dynamic Screw

PATENT NUMBER  
Dynamic Screw  
EP 2 932 937

## High Dynamic Screw


Dynamic screws cover all the thread metrics available on the market. They are used with the Dynamic TiBase® or milled structures with an angled screw channel. There are several lengths for each metric to ease adaptation to the structures.

All of them are made of Titanium grade V.

All screws are perfectly identified with their batch and reference numbers, which allow each and every screw to be traced and recorded in the patient's card and in the clinical or laboratory records. Only the 3.0 dynamic screwdriver must be used to install them.

# DAS PRODUCTS

# CAD-CAM WORKFLOW

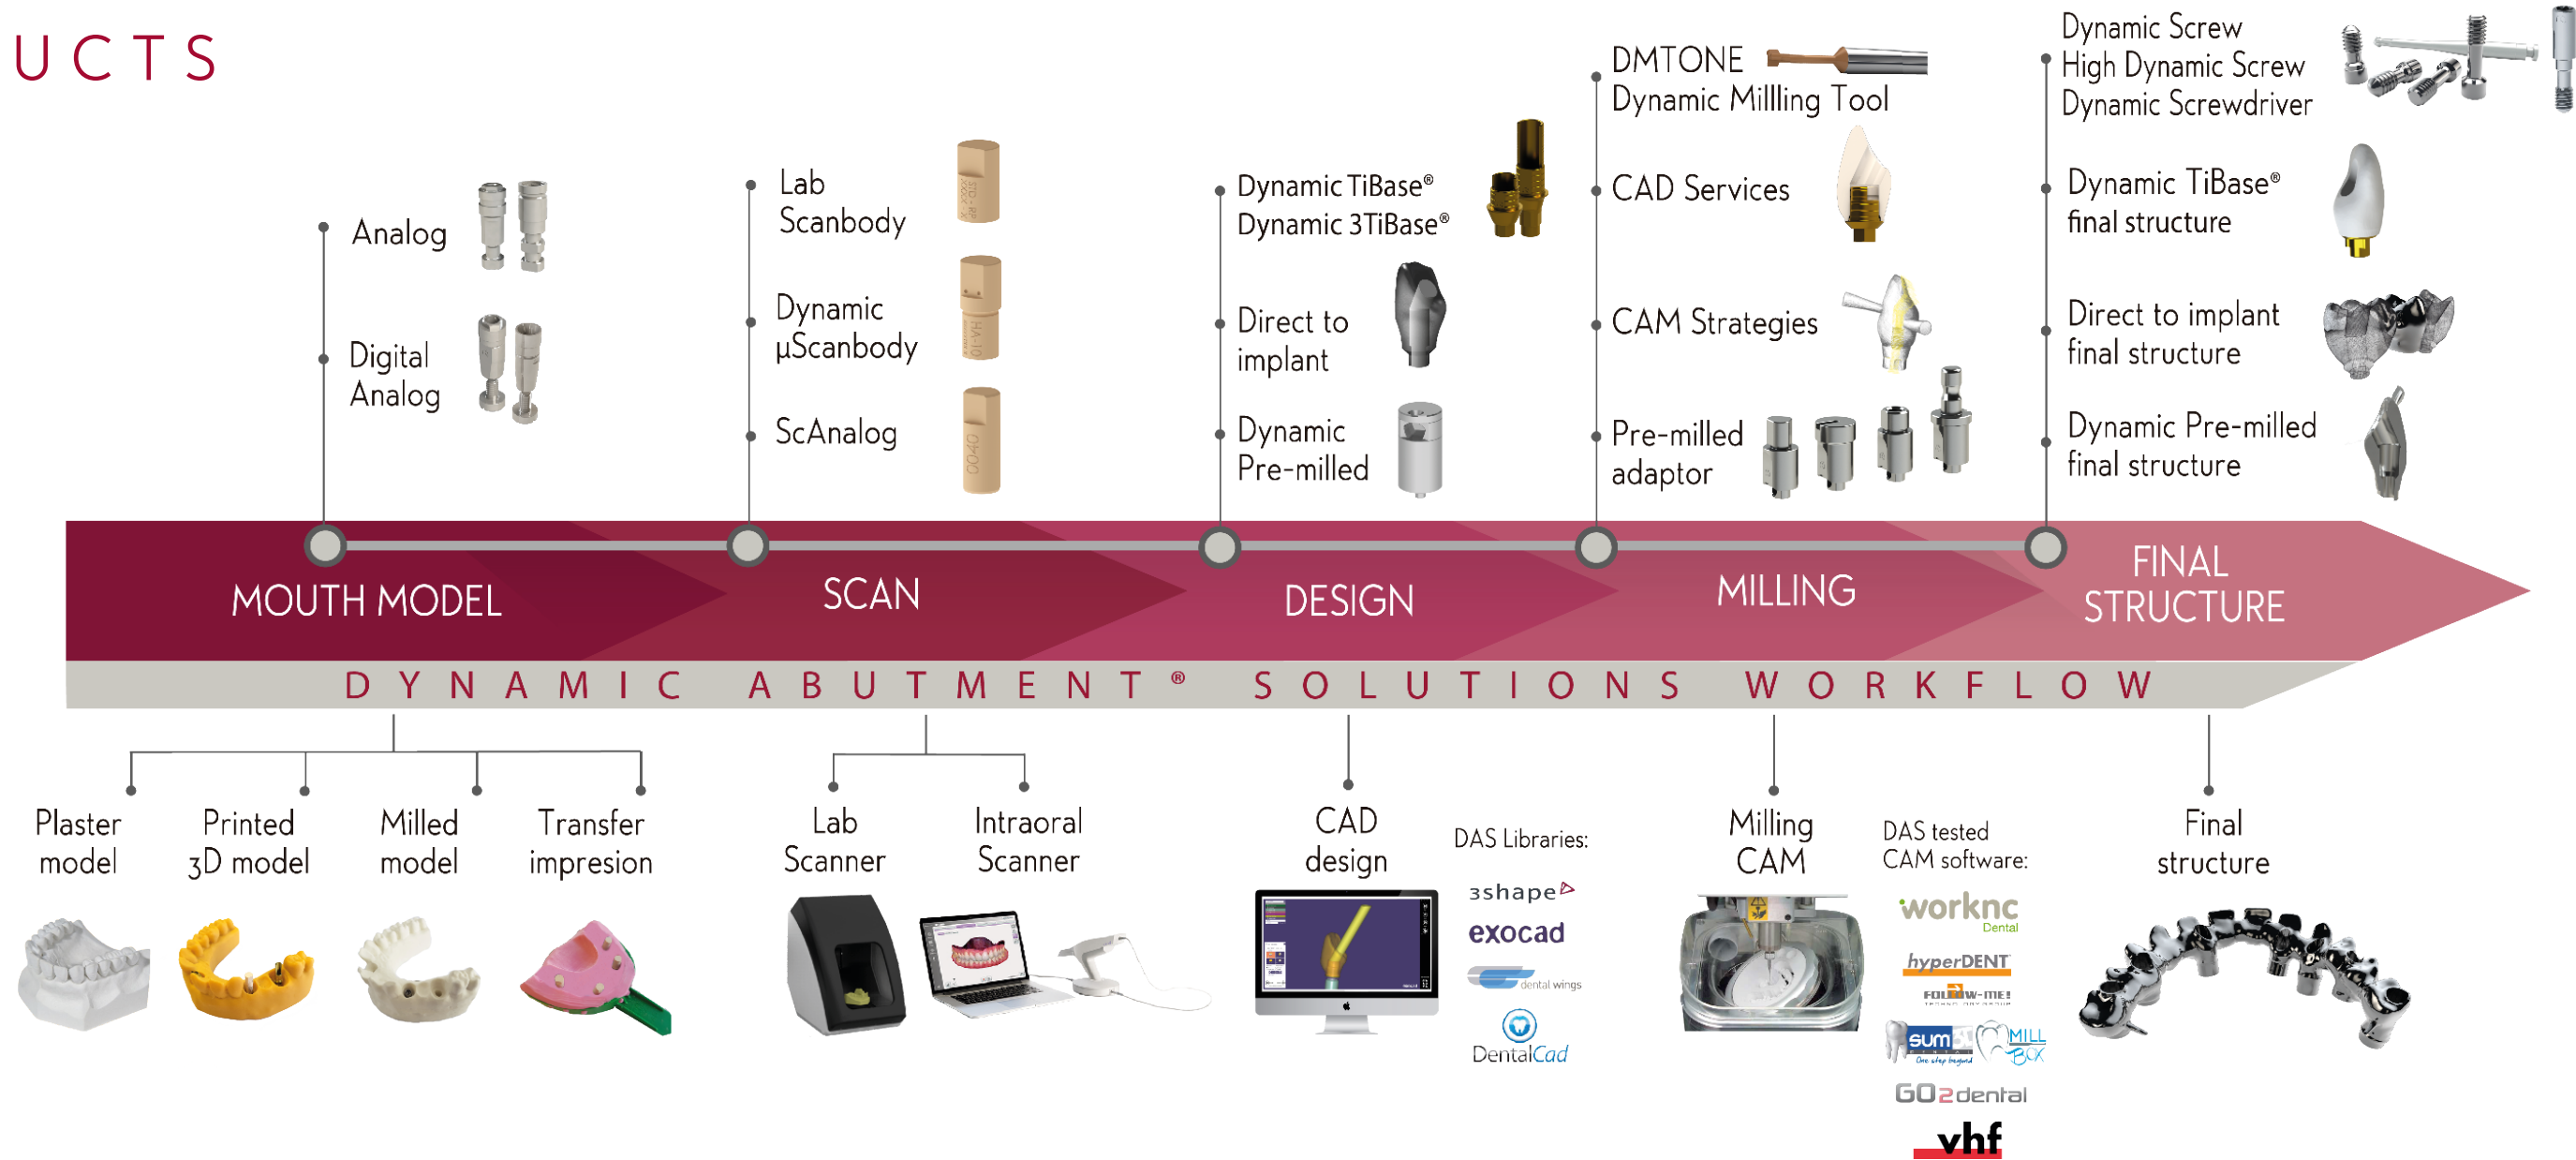



# DYNAMIC μSCANBODY

The scanbody detects the position and orientation of the respective dental implant or analog in CAD-CAM scanning procedures.


## Hole free scanbody and not screwed

There are no holes in the upper section which means the Z axis is free to improve scanbody scanning.

The angulation of the chimney it goes always on the opposite side of the scanbody lateral cut.

The diameter of the scanbody is always equal or smaller than the implant diameter.



**3 lengths**  
(8mm, 10mm and 12mm) for the most complex scanbody reading cases.

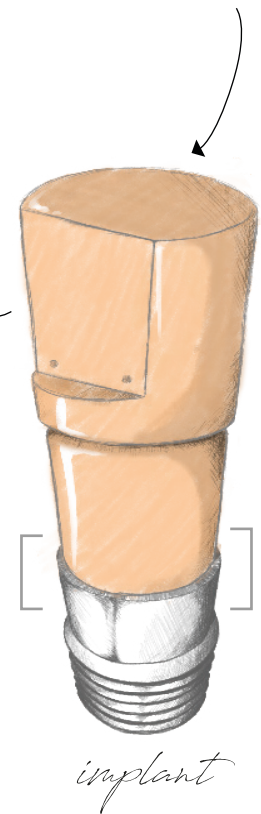

# ADAPTOR

Connecting element between the scanbody and the implant. Marked with different colors according to the compatibility\*

\*See pages 162 to 165

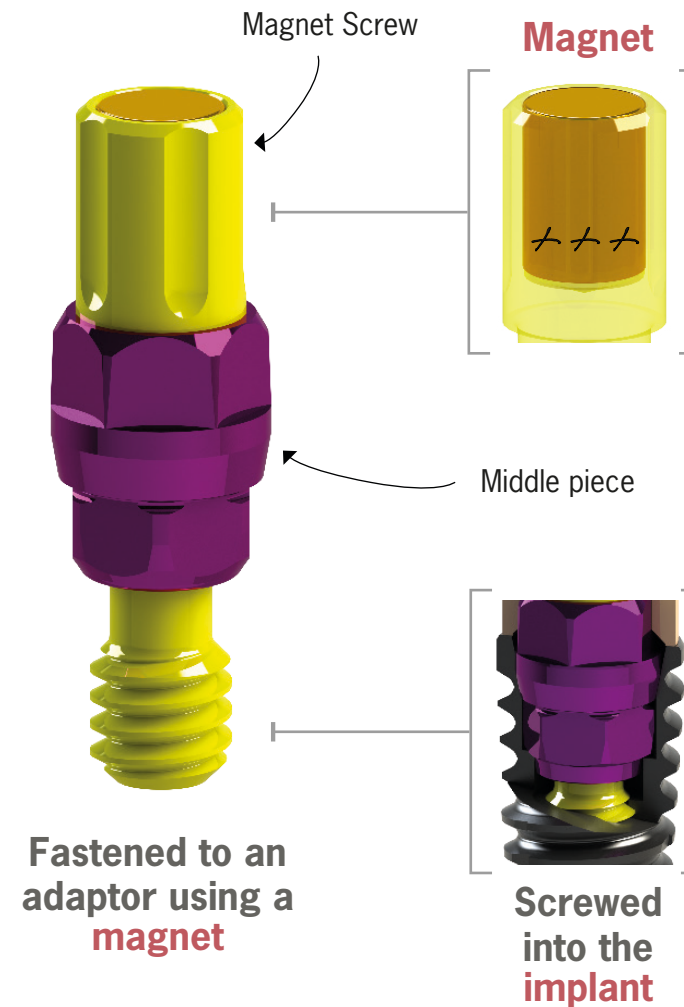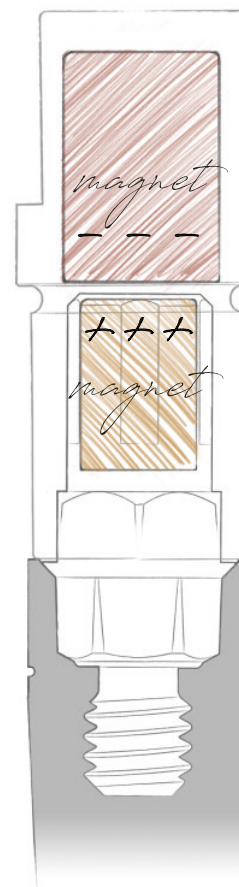


Special screwdriver for the adaptor\*  
\*See page 168




# LAB SCANBODY


Only for Dynamic TiBase® and Lab Scanner

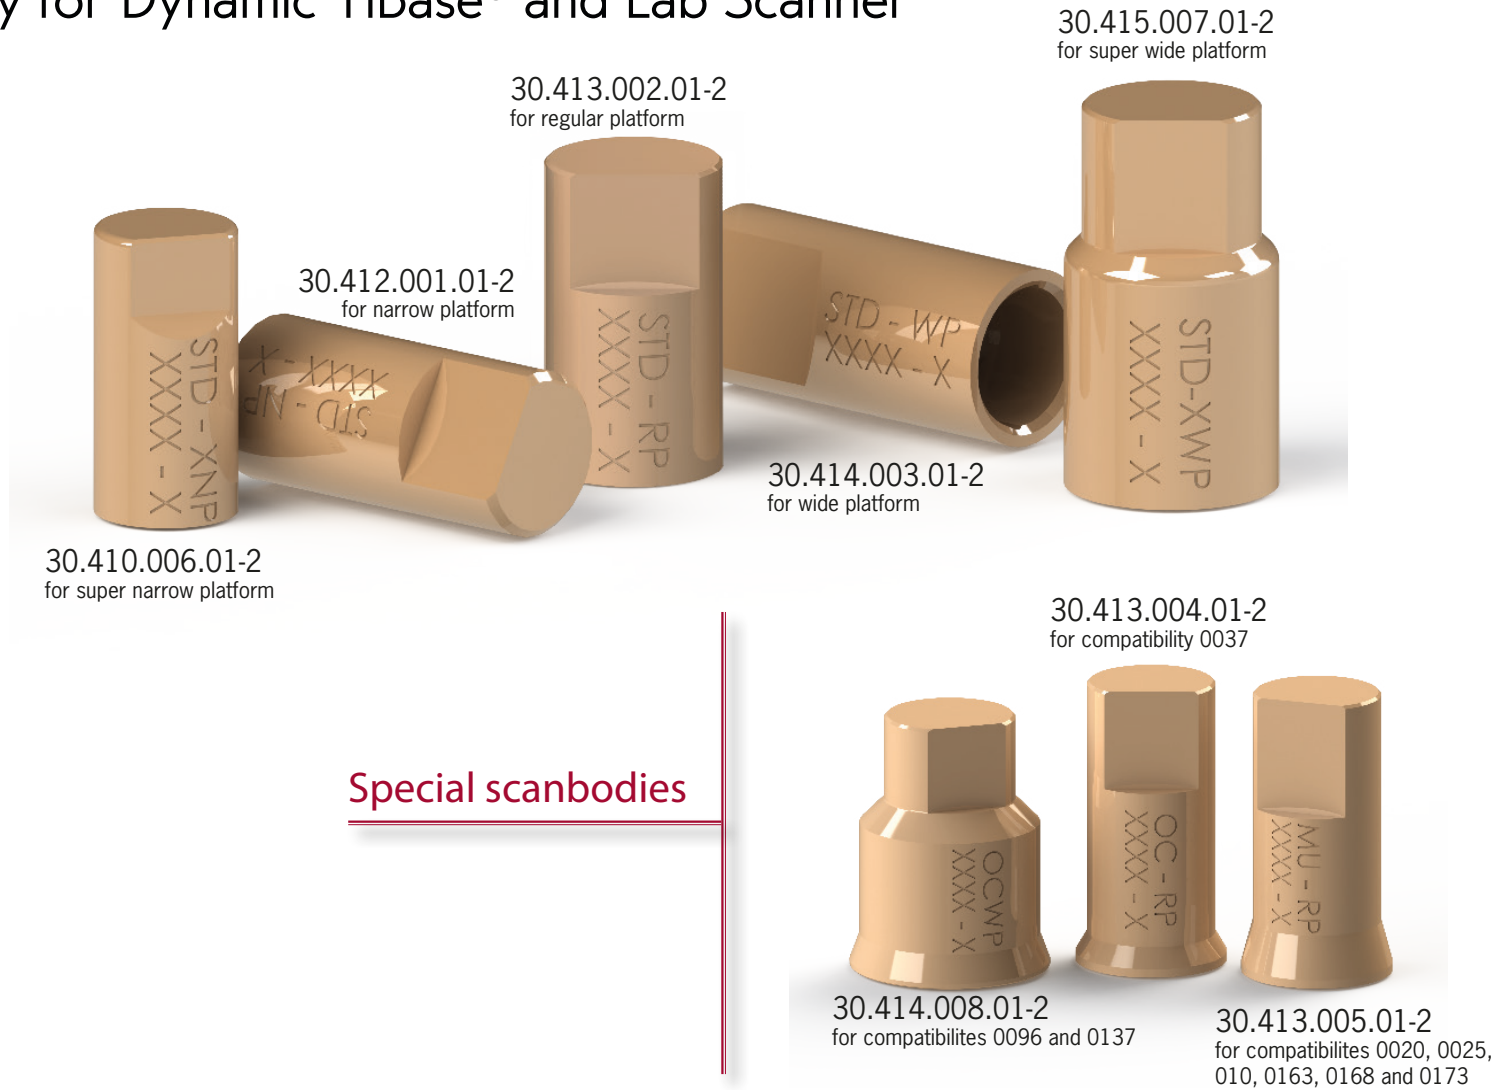

## Special scanbodies

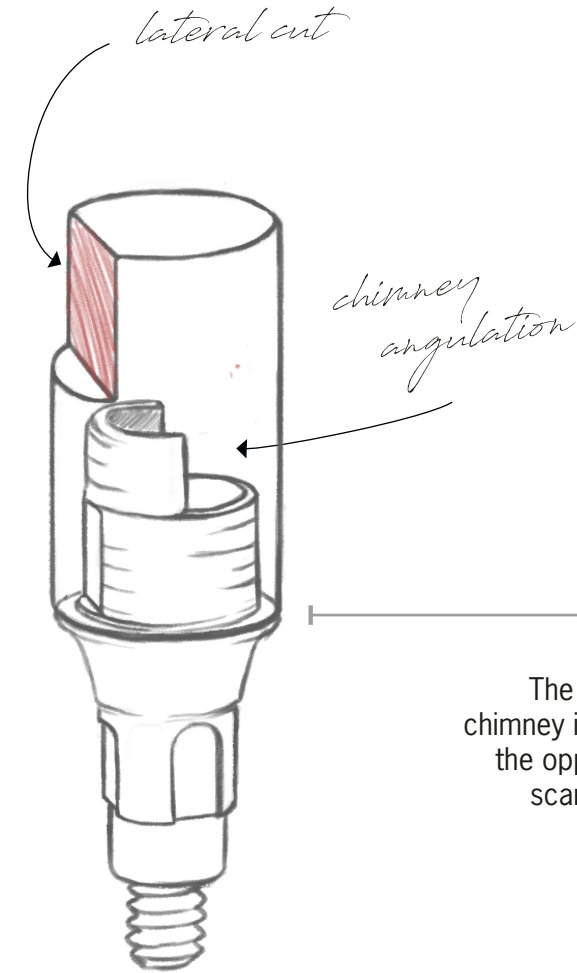

**Perfect fit**  
The angulation of the chimney it goes always on the opposite side of the scanbody lateral cut.

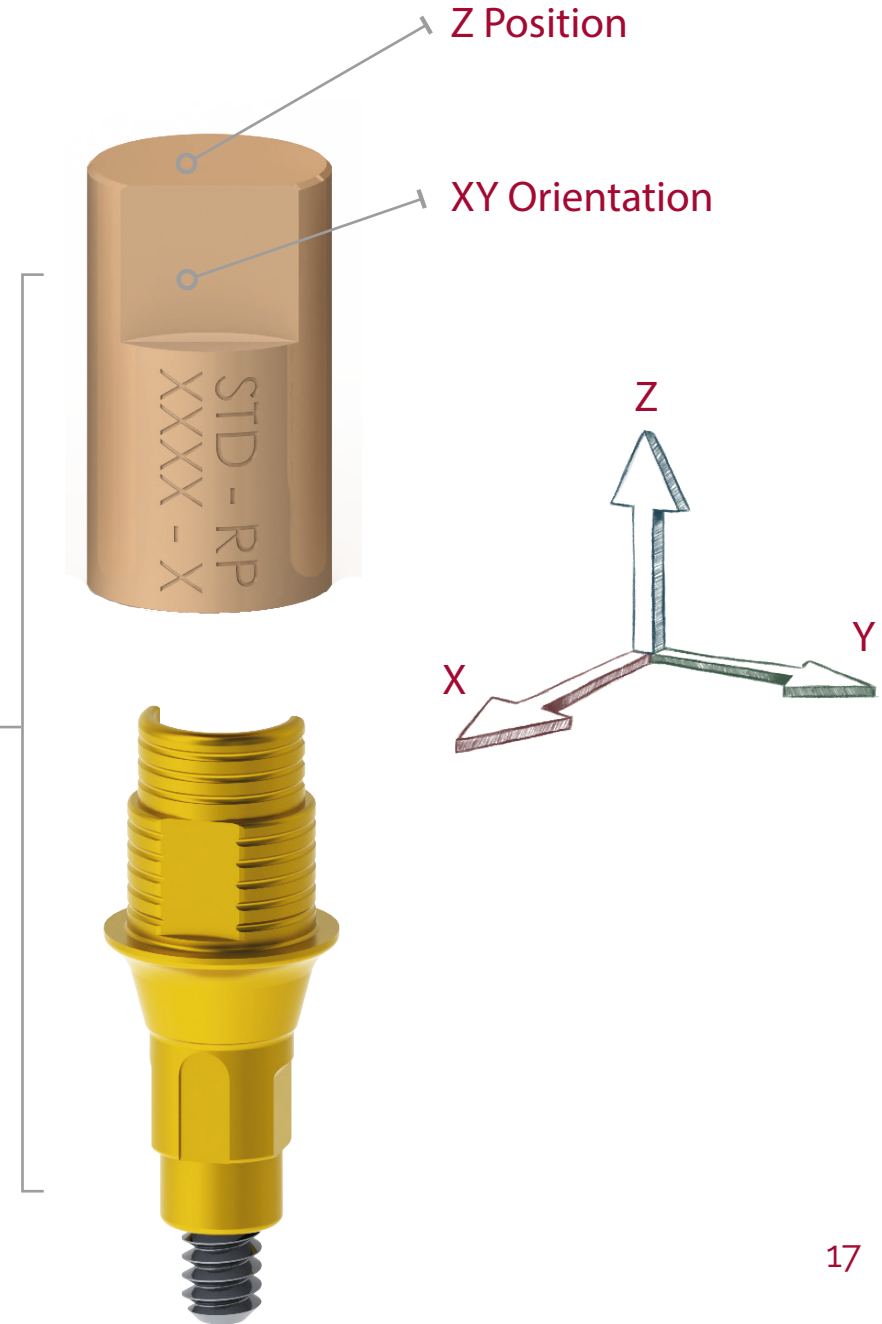



# DYNAMIC TIBASE® \*

Dynamic TiBases® are a technological contribution to the digital treatment for the angled systems development using CAD-CAM: the Dynamic System includes the Dynamic TiBase®, the dynamic screw-screwdriver set, scanbodies and digital libraries available for the main CAD softwares on the market: Exocad, 3Shape, Dentalwings and Dental Cad.

PATENT NUMBER  
Dynamic TiBase®  
US 10.130.447

TO CORRECT  
ANGULATION

up to  
45°




Dynamic screw

Straight screw

\*Maximum angulation available for the first TiBase gingival height. Maximum angulations for the rest of gingival heights under development

Our grade V titanium bases are **gold anodized** to improve the work's aesthetic.

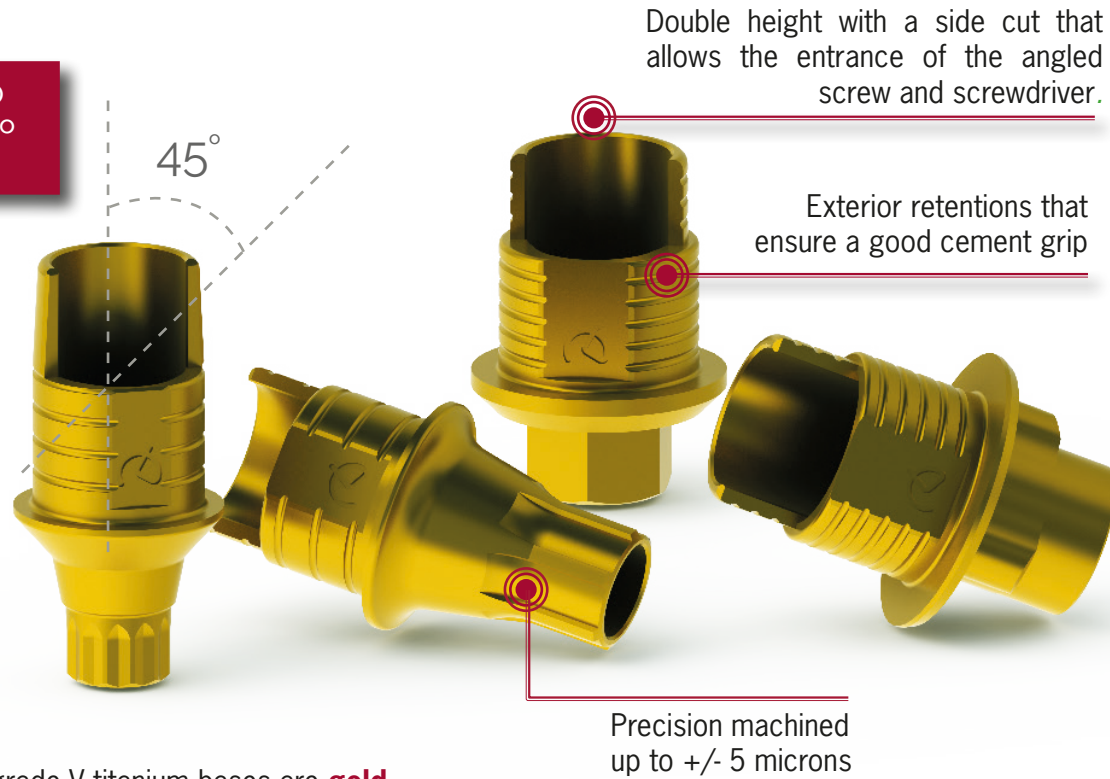


Double height with a side cut that allows the entrance of the angled screw and screwdriver.

Exterior retentions that ensure a good cement grip

Precision machined up to +/- 5 microns

# DYNAMIC 3TIBASE®

The Dynamic 3TiBase® offers the possibility to work with different cement heights: 5, 7 or 9mm. It is specially designed for the cases that require higher height. In this way, a greater support surface is achieved, the structure is stronger and more resistant so structure breaks by height decompensation between the TiBase and the structure are avoided.

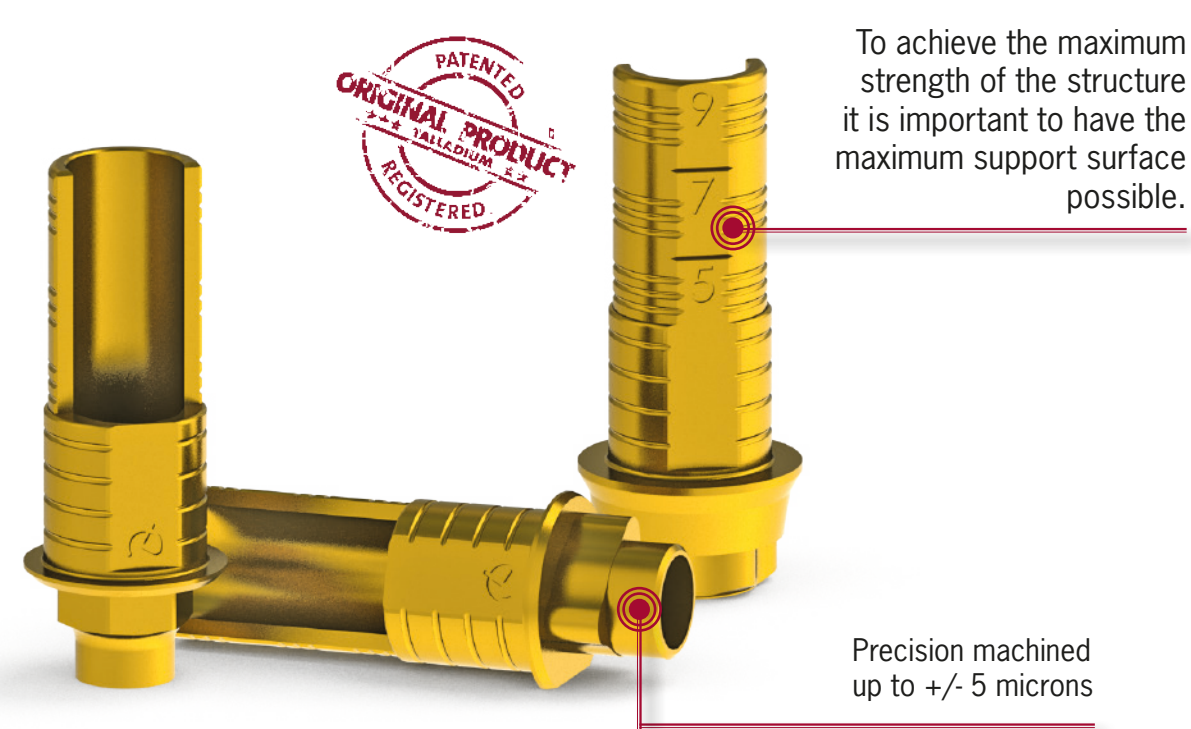

PATENTED  
ORIGINAL PRODUCT  
REGISTERED

To achieve the maximum strength of the structure it is important to have the maximum support surface possible.

Precision machined up to +/- 5 microns




Scan with the Dynamic μScanbody and cement the final piece onto the 3TiBase.



If you do not have the Dynamic μScanbody, it is necessary to use the 4mm TiBase and the Lab scanbody to make the scanning. The final piece is cemented onto the 3TiBase.

# DYNAMIC TIBASE®

*Gingival options*

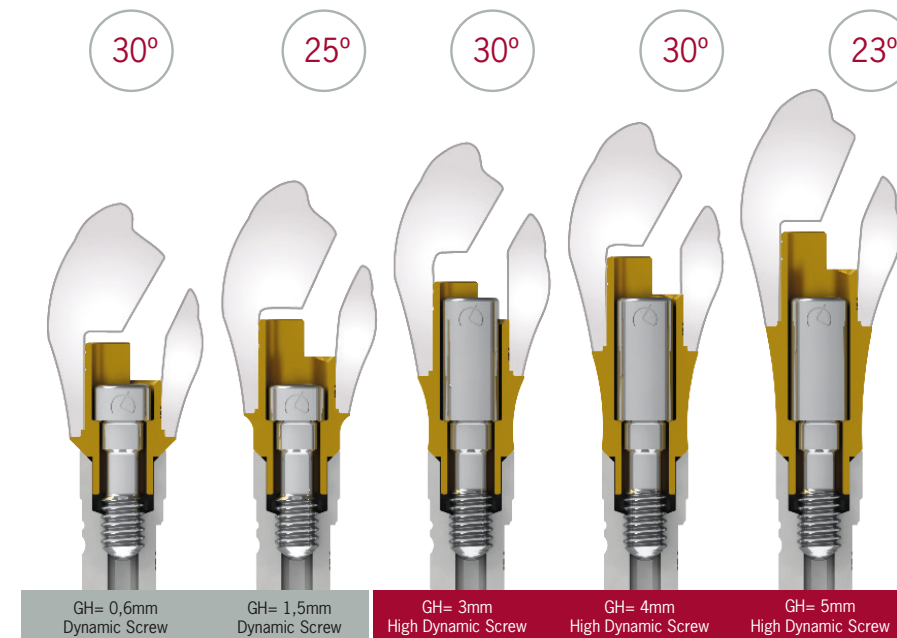

\*Example with TiBase® compatible with Zimmer Screw-Vent Ø3,5 (Code 0040)



- Keep the angulation
- Best aesthetic angled channel Ø 2mm
- Angled channel reduction of 32%
- Increases the volume of the structure
- Captive Screw

(Put the screw on the TiBase® before cementing)






Ø 12

# DYNAMIC PRE-MILL3D®


PATENT NUMBER  
Dynamic Premilled  
ES 2590002

**DYNAMIC  
PREMILL3D**  
DYNAMIC ABUTMENT® SOLUTIONS



### Pre-milled angled channel

The Dynamic Premill3d® already comes with a pre-milling of the inner channel



### Angulation from 0 to 30° choice

Allows to choose angulation of the screw channel on the CAD for the later insertion of the screw



### Milling of the angulated screw channel

CAD design and milling of the angled channel on CAM by the customer



### Dynamic Pre-milled final structure


### Available in Cobalt-Chrome

Allows to apply ceramic directly

Optimized for a better milling strategy



Precision machined up to +/- 5 microns

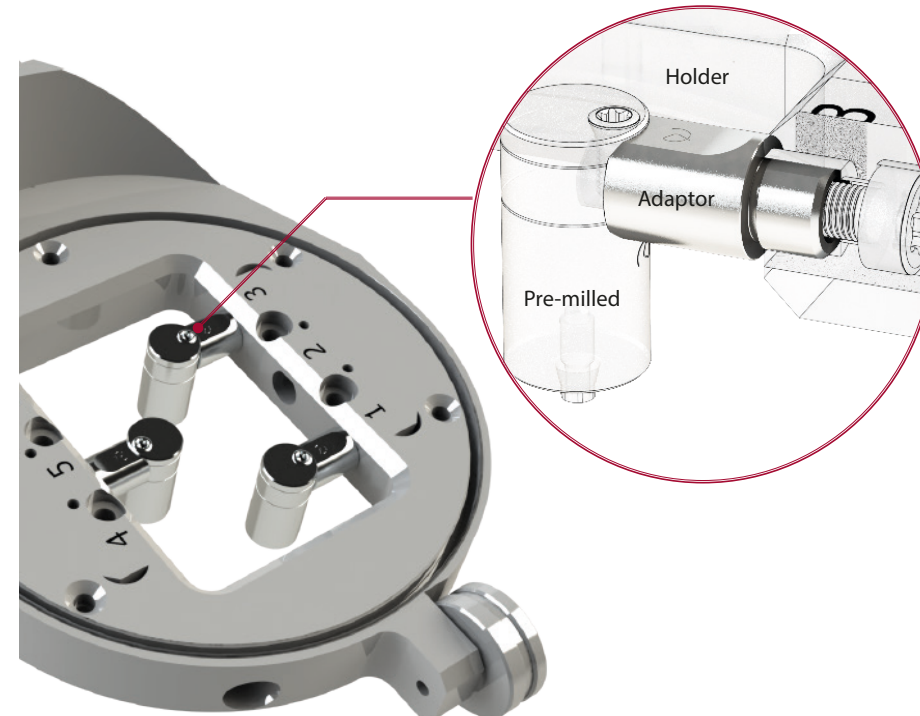

# ADAPTORS



Ref: 39.903.001.01-2


Ref: 39.903.002.01-2

Ref: 39.903.003.01-2

Ref: 39.903.008.01-2

### It is not necessary to purchase a new holder

The adapter has the holder connection and connects the holder to the pre-milled abutment.

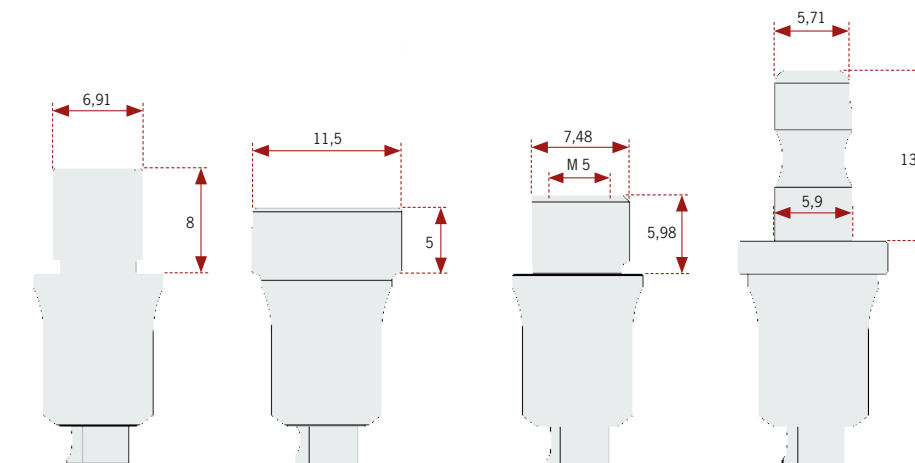

## Customized ADAPTORS


We design and manufacture the adapter for any type of adaptor (das@dynamicabutment.com)

# DYNAMIC MILLING TOOL

Each tool is compatible depending on **screw seating, metric and length**




Shank  
Ø3, Ø4, Ø6

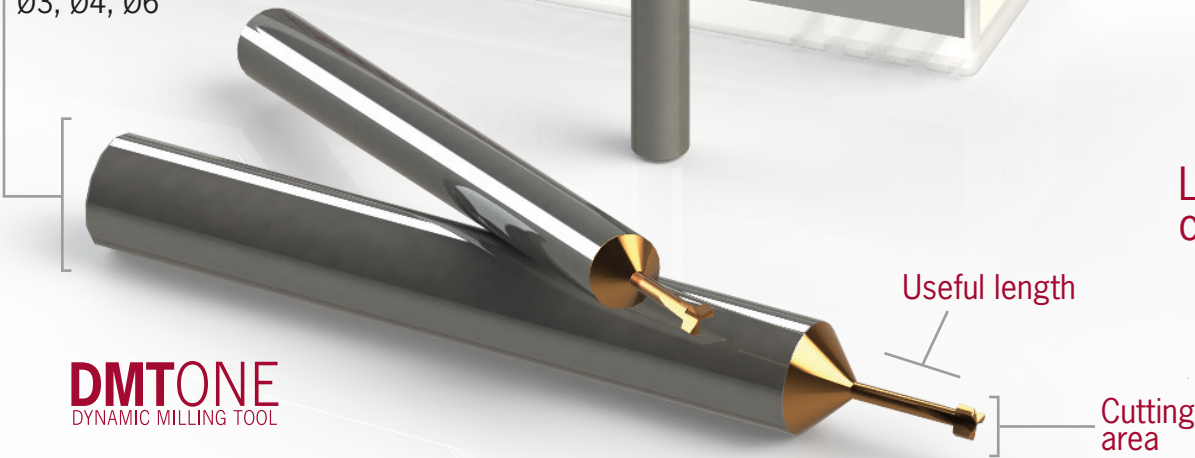


## DIRECT TO IMPLANT (one piece) and ANGULATED

Precision milling tool. In the screwed angled structure direct to implant, it is used to mill the screw seating and to increase the internal diameter of the straight channel.


There are 3 cutting wing-tips with 3 different cutting area each, to mill the screw seating and to increase the internal diameter of the straight channel.

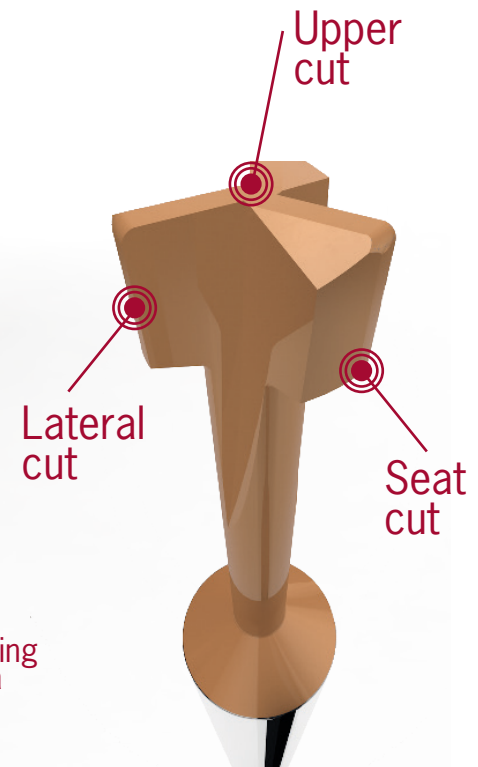


PATENT NUMBER  
Milling process of the  
angulated channel  
ES 2658 985




**STEP 1:**  
Crown with pre drill.



**STEP 2:**  
Crown with Angled channel.

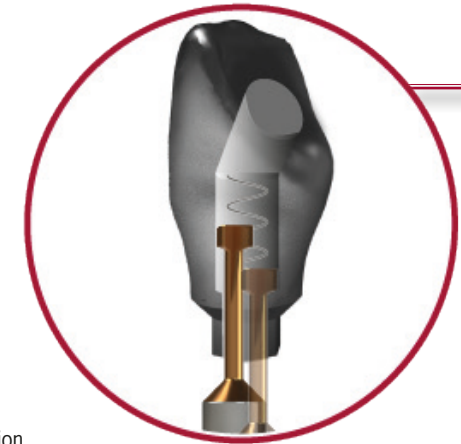


**STEP 3:**  
Crown with Dynamic Milling Tool.  
Milling the screw seat and increasing the diameter of the straight channel.

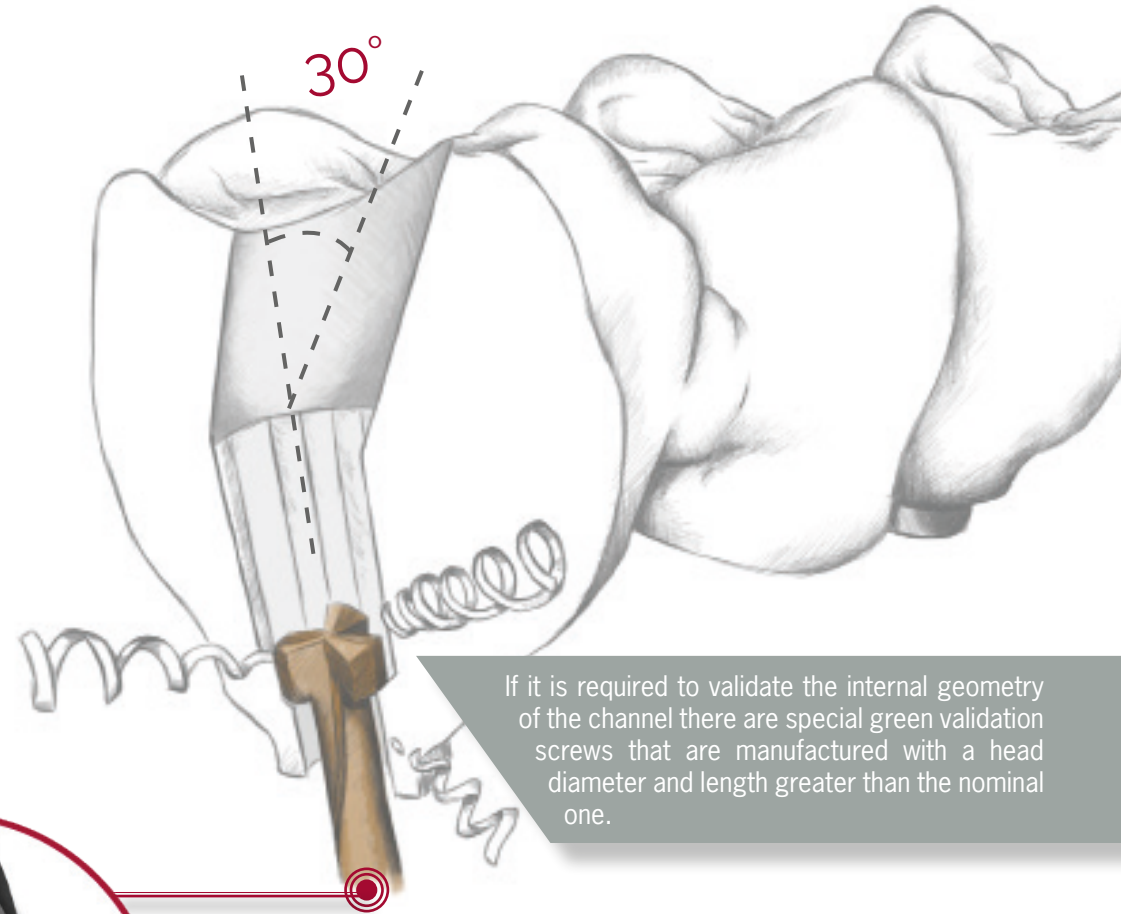

If it is required to validate the internal geometry of the channel there are special green validation screws that are manufactured with a head diameter and length greater than the nominal one.

**TESTED and VALIDATED by**



\*Direct to implant maximum angulation under development



# DIGITAL ANALOG

Digital analog of the dental implant to simulate implant position in a 3D printed dental model.




## 3D PRINTED MODEL


The dental model - for later insertion of the analogs - is designed using the CAD libraries.



3shape  
Model Builder




exocad  
Model Creator




dental wings  
Model Builder



**Concave notch**  
Top precision in longitudinal position



**Curved Surface**  
Accuracy of orientation guaranteed





**Longitudinal cut**  
Longitudinal cut to avoid rotation X-Y

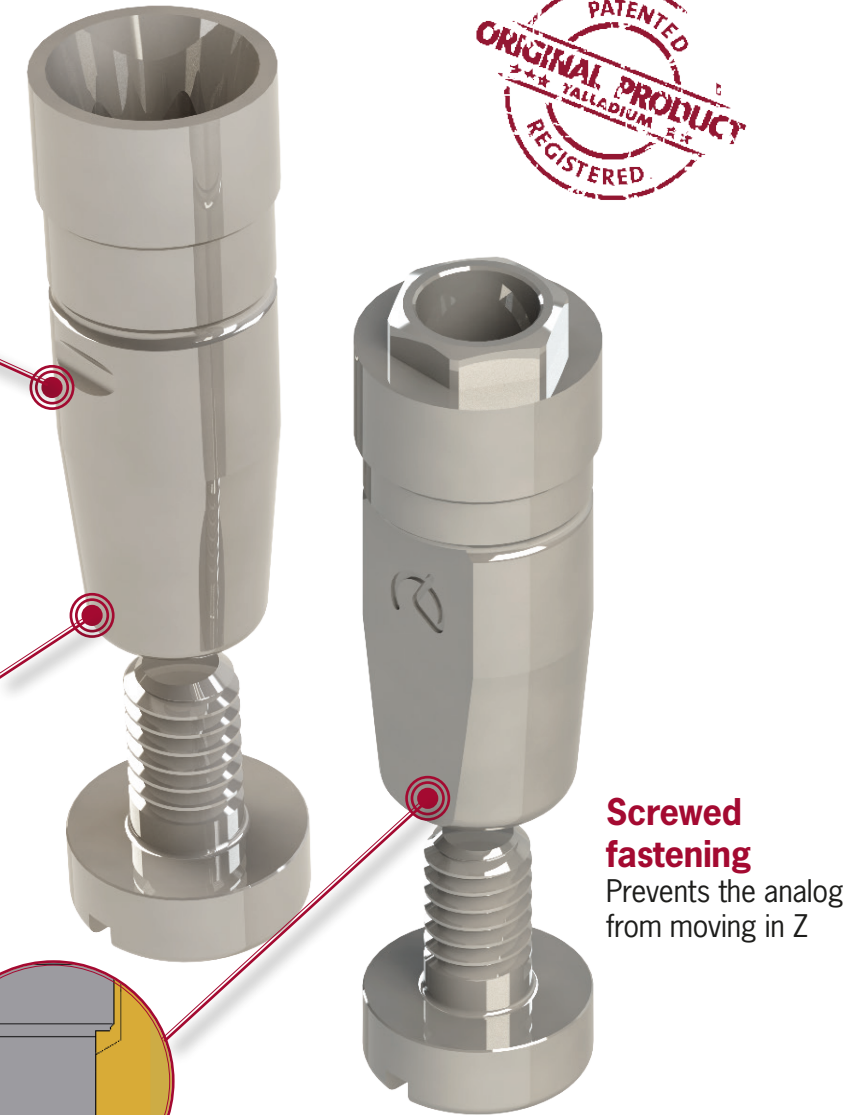

**Screwed fastening**  
Prevents the analog from moving in Z



# DAS LIBRARIES

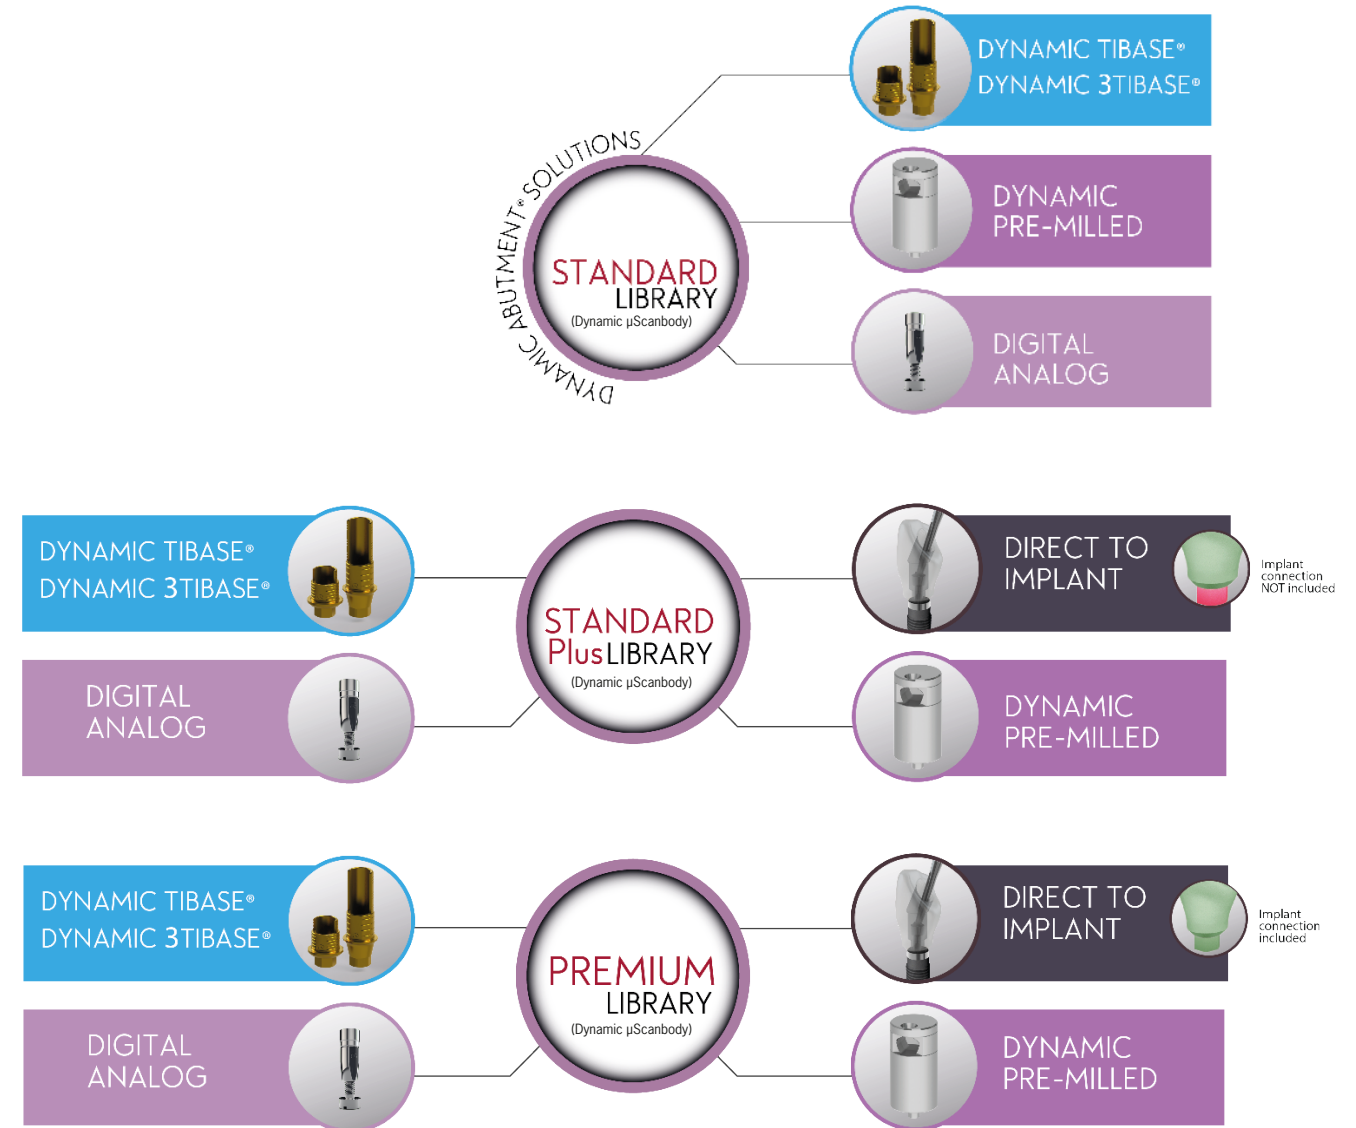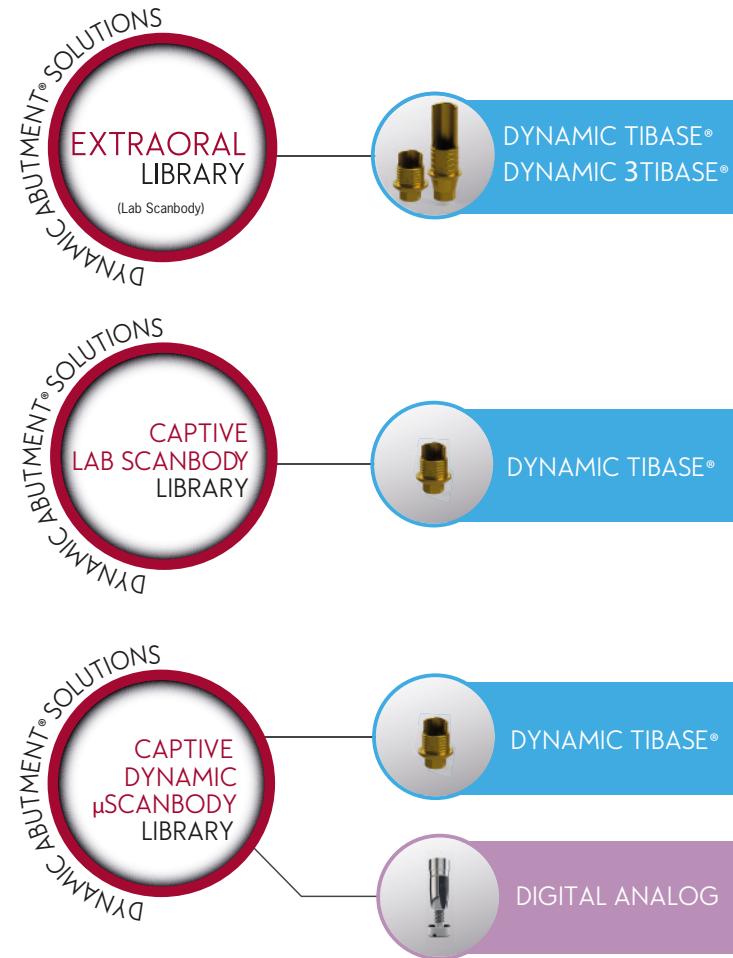


# DAS CUSTOMIZE SERVICES

## PRODUCT DEVELOPMENT


Any DAS traded goods can be made-to-measure or adapted to your work protocol. DAS complements the development of new products with the technological support (software, libraries, tools, etc.) necessary, alongside all the guarantees any healthcare product needs.

## CAD ADAPTION SERVICES

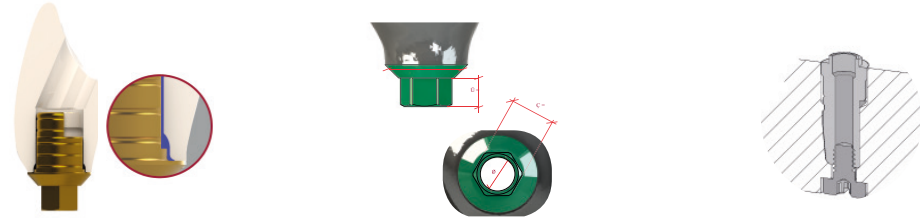

- ✦ Adjustment of the CAD libraries for our products to client needs: angled channel diameter modification, calibration of cemented gap TiBase®, adjustment of 3D digital analog printing gap, etc.
- ✦ CAD libraries supplied with implant connections; DAS currently has over 500 implant compatibilities.
- ✦ Development of special CAD libraries for connections pertaining to the client.
- ✦ Design of libraries linked to client's specific scanbodies.
- ✦ Etc.

## CAM SUPPORT and ADVICE

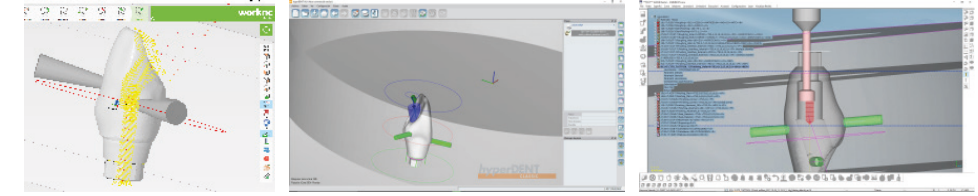

Dynamic Abutment® Solutions products have been tested and validated by the leading CAM software brands on the market.

- ✦ Provision of implant connections with nominal values.
- ✦ Design and production of special tools to mill connections or special geometries (abutments).
- ✦ Design and production of special supports for your milling equipment: pre-milled supports, etc.
- ✦ Technology for machining angled channels (copyright-free).






## SPECIALIZED CONSULTANCY



Multidisciplinary experience in different areas of dental research and regular collaboration on projects with the key operators in the sector have provided us with experience and know-how that we want to make available to you, so we can advise you, work together and pursue customized projects. All DAS technological and human resources are available to help turn your idea into a reality, providing expert advice and support throughout all the developmental stages.

# DYNAMIC TIBASE®

CAD








3shape

exocad

dental wings

DentalCad

CAM



Tested CAM Software

worknc  
Dental

FOLLOW-ME!  
TECHNOLOGY GROUP


sum31  
DENTAL  
One step beyond

MILL  
BOX


GO2dental  
cam for dental labs

vhf

# DIRECT to IMPLANT

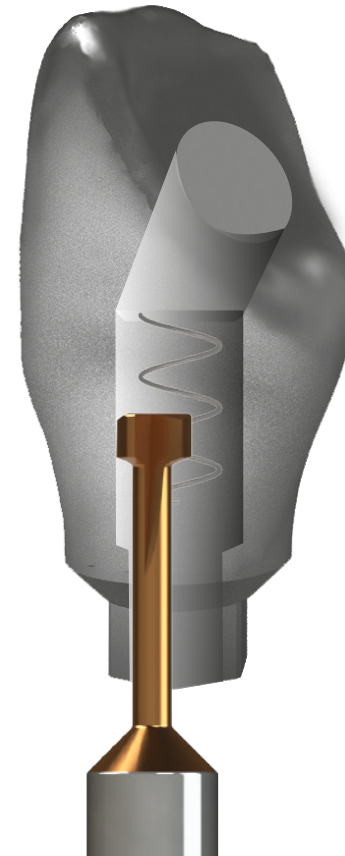


CAD

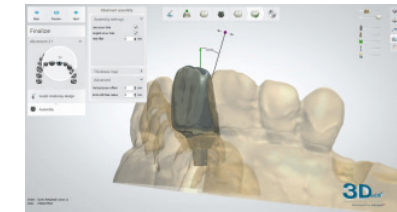

3shape




exocad

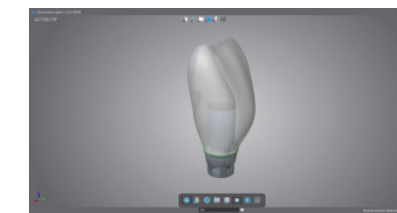


dental wings


CAM

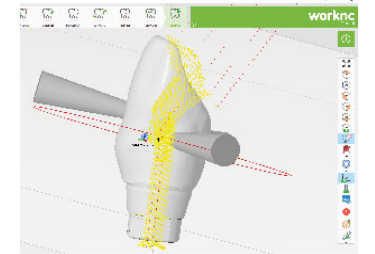

worknc  
Dental

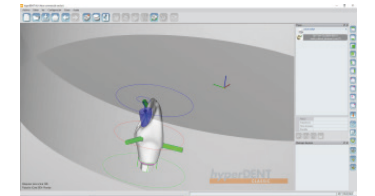

FOLLOW-ME!  
TECHNOLOGY GROUP

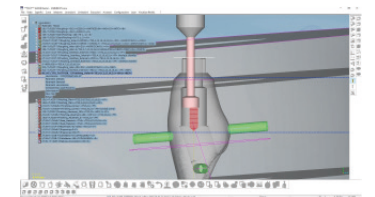


sum31  
DENTAL  
One step beyond

MILL  
BOX


# DIGITAL ANALOG




## CAD-CAM

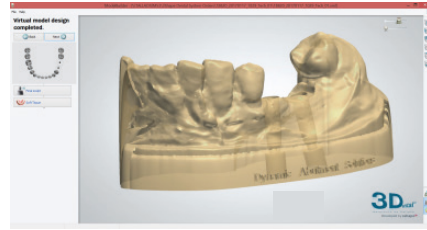

**3shape**   
Model Builder

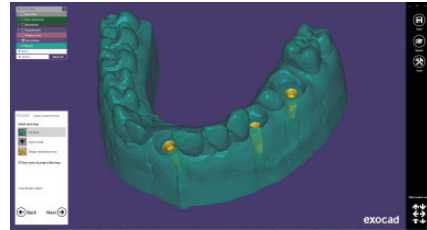

**exocad**  
Model Creator

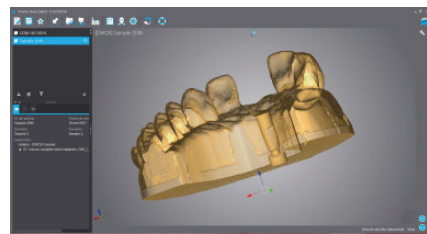


 **dental wings**  
Model Builder


# DYNAMIC PRE-MILL3D®




## CAD

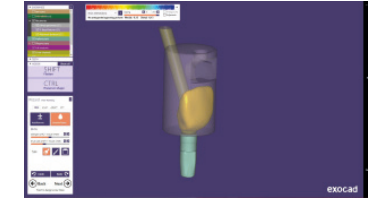

**exocad**

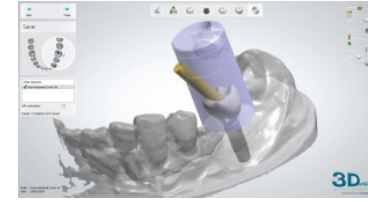


**3shape** 




 **dental wings**

## CAM

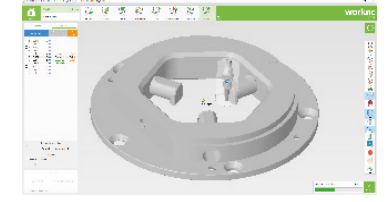

**worknc**  
Dental

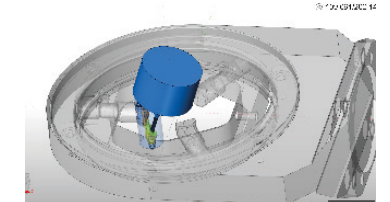

**sum31**   
DENTAL *One step beyond*

 **FOLLOW-ME!**  
TECHNOLOGY GROUP

\*Soon



# DYNAMIC SYSTEM



# List of compatibilities available

AB  
ACE  
ADIN  
ALPHABIO  
ANCLADEN  
ANKYLOS  
ANTHOGYR  
ARDS  
ASTRA  
AVINENT  
BEGO  
BIOCONCEPT  
BIOGENESIS  
BIOHORIZONS  
BIOMET 3i  
BIOLOK  
BIONER  
BIOTEC  
BIOTECH  
BREDENT MEDICAL  
BTI  
BTK  
B&W  
CAMLOG  
CONEXÃO SISTEMA DE PRÓTESE  
CORTEX  
DENTAL TECH  
DENTAURUM  
DENTIS  
DENTIUM

DIO IMPLANTS  
DSP BIOMEDICAL  
EASY IMPLANT  
ECKERMANN  
ELITE MEDICA  
EUROTEKNIKA  
GALIMPLANT  
GMI (ILERIMPLANT)  
GT MEDICAL  
HAHN IMPLANT (GLIDEWELL)  
HI-TEC  
IDO IMPLANTS  
IHDE DENTAL (IMBIODENT)  
IMPLANT DIRECT  
IMPLANT GENESIS  
INTRA-LOCK  
JDENTALCARE  
KEYSTONE  
KLOCKNER  
LASAK  
LEADER  
MEDENTIS  
MEGAGEN  
MICRODENT  
MIS  
MOZO-GRAU  
MPI  
NEOBIOTECH  
NEODENT  
NEOSS

NOBEL BIOCARE  
NORIS MEDICAL  
NORMON  
NOVA IMPLANTS  
OSSTEM IMPLANT  
OSTEOPLUS  
PALTOP  
PHIBO  
PROCLINIC  
RADHEX  
SEWON MEDIX  
SGS  
SIGNO VINCES  
SOUTHERN IMPLANTS  
STERNGOLD  
STRAUMANN  
SWEDEN & MARTINA  
SYBRON IMPLANT SOLUTIONS  
TITANIUM - FIX  
TRE-OSS  
TRI DENTAL IMPLANTS  
TRINON  
UFIT  
VULKAN IMPLANTS  
XIVE  
YES IMPLANT  
ZIACOM (OSSEOLIFE)  
ZIMMER



## AB

- ✦ I2  
Implant: Ø 3,5/3,75/4,2/4,5/ 5/6  
Platform: Standard (Code 0040) p. 89
- ✦ I22  
Implant: Ø 3,75/4,22  
Platform: Standard (Code 0040) p. 89
- ✦ I5  
Implant: Ø 3,5/3,75/4,2/4,5/5/6/7/8  
Platform: Standard (Code 0040) p. 89
- ✦ I55  
Implant: Ø 3,75/4,2/4,5/5/6/7/8  
Platform: Standard (Code 0040) p. 89
- ✦ I10  
Implant: Ø 4,2/5  
Platform: Standard (Code 0040) p. 89
- ✦ I15  
Implant: Ø 6/7/8  
Platform: Standard (Code 0040) p. 99
- ✦ Multi Unit D1-P64  
Platform: Universal (Code 0025) p. 76

## ACE

- ✦ External Hex  
Implant: Ø 3,3  
Platform: NP 3,5 (Code 0023) p. 74  
Implant: Ø 3,75/4  
Platform: RP 4,1 (Code 0024) p. 75  
Implant: Ø 4,75  
Platform: WP 5 (Code 0058) p. 104

## ✦ Infinity TRI-CAM

- Implant: Ø 3,5  
Platform: 3,5 (Code 0026) p. 77
- Implant: Ø 4,3  
Platform: 4,3 (Code 0027) p. 78
- Implant: Ø 5  
Platform: 5 (Code 0028) p. 79

## ✦ Infinity Internal Hex

- Implant: Ø 3,7/4,1  
Platform: 3,5 (Code 0040) p. 89
- Implant: Ø 4,7/5,1  
Platform: 4,5 (Code 0041) p. 91

## ✦ Infinity Octagon

- Implant: Ø 3,3/4,1/4,8  
Platform: RP 4,8 (Code 0037) p. 86
- Implant: Ø 4,8  
Platform: WP 6,5 (Code 0096) p. 122

## ✦ Multi Unit

- Platform: Universal (Code 0025) p. 76

## ADIN

### ✦ Swell

- Implant: Ø 3,3  
Platform: 3,45 (Code 0040) pg. 89
- Implant: Ø 3,75/4,2  
Platform: 3,6 (Code 0040) pg. 89
- Implant: Ø 5  
Platform: 4 (Code 0040) pg. 89
- Implant: Ø 6  
Platform: 4,6 (Code 0040) pg. 89

## ✦ Touareg-S / Touareg-OS

- Implant: Ø 3,5  
Platform: 3,45 (Code 0040) p. 89
- Implant: Ø 3,75/4,2  
Platform: 3,6 (Code 0040) p. 89
- Implant: Ø 5  
Platform: 4 (Code 0040) p. 89
- Implant: Ø 6  
Platform: 5 (Code 0040) p. 89

## ✦ Touareg CloseFit

- Implant: Ø 3,5  
Platform: RP (Code 0021) p. 72
- Implant: Ø 4,3/5  
Platform: WP (Code 0022) p. 73

## ✦ Multi Unit TMA

- Platform: Universal (Code 0025) p. 76

## ALPHABIO

### ✦ Internal Hex Connection (IH) SPI

- Implant: Ø 3,3/3,75/4,2/5/6  
Platform: Universal (Code 0040) p. 89

### ✦ Internal Hex Connection (IH) ICE

- Implant: Ø 3,7/3,75/4,2/4,65/5,3  
Platform: Universal (Code 0040) p. 89

### ✦ Internal Hex Connection (IH) DFI

- Implant: Ø 3,3/3,75/4,2/4,5  
Platform: Universal (Code 0040) p. 89

### ✦ Internal Hex Connection (IH) ATID

- Implant: Ø 3,3/3,75/4,2/5/6  
Platform: Universal (Code 0040) p. 89

### ✦ Internal Hex Connection (IH) NEO

- Implant: Ø 3,75/4,2/5  
Platform: 3,5 (Code 0040) p. 89

## ✦ Conical Hex Connection (CHC) NICE

- Implant: Ø 3,2  
Platform: Narrow (Code 0136) p. 137

## ✦ Conical Hex Connection (CHC) NEO

- Implant: Ø 3,2/3,5  
Platform: Narrow (Code 0136) p. 137

## ✦ Conical Standard Connection (CS)

- Implant: Ø 3,75/4,2/5  
Platform: Standard (Code 0169) p. 151

## ANCLADEN

### ✦ Anclalock

- Implant: Ø 3,75/4,25/5  
Platform: 3,5 (Code 0040) p. 89

## ANKYLOS

### ✦ Ankylos

- Implant: Ø 3,5  
Platform: 3,5 (Code 0075) p. 113
- Implant: Ø 4,5  
Platform: 4,5 (Code 0075) p. 113
- Implant: Ø 5,5  
Platform: 5,5 (Code 0075) p. 113
- Implant: Ø 7  
Platform: 7 (Code 0075) p. 113

## ANTHOGYR

### ✦ Axiom REG / PX

- Implant: Ø 3,4  
Platform: 3,4 (Code 0161) p. 143
- Implant: Ø 4  
Platform: 4 (Code 0149) p. 139
- Implant: Ø 4,6  
Platform: 4,6 (Code 0149) p. 139
- Implant: Ø 5,2  
Platform: 5,2 (Code 0162) p. 144

## ✦ Anthofit HE

- Implant: Ø 3,5/3,75/4  
Platform: R (4,1) (Code 0024) p. 75
- Implant: Ø 5  
Platform: L (5) (Code 0058) p. 104

## ✦ Ossfit

- Implant: Ø 3,5/4,2  
Platform: 4,8 (Code 0074) p. 112
- Implant: Ø 3,5/4,2  
Platform: 4,8 (Code 0037) p. 86
- Implant: Ø 5  
Platform: 6,5 (Code 0096) p. 122

## ✦ Multi Unit

- Implant: Ø 4,8  
Platform: Universal (Code 0163) p. 145

## ARDS

### ✦ Smart

- Implant: Ø 3,75/4,2/4,5  
Platform: 3,75 (Code 0040) p. 89

### ✦ Classic

- Implant: Ø 3,75/4,2/4,5  
Platform: 3,75 (Code 0040) p. 89
- Implant: Ø 3,3/3,75/4,2/5/6  
Platform: 3,75 (Code 0040) p. 89

### ✦ Premium

- Implant: Ø 3,3/3,75/4,2/5/6  
Platform: 3,75 (Code 0040) p. 89

### ✦ CIT

- Implant: Ø 3,3/3,75/4,2/5/6  
Platform: 3,75 (Code 0040) p. 89

## ASTRA

### ✦ Yellow

- Implant: Ø 3  
Platform: Yellow (Code 0109) p. 125

### ✦ Aqua

- Implant: Ø 3,5/4  
Platform: Aqua (Code 0004) p. 55

### ✦ Lilac

- Implant: Ø 4,5/5  
Platform: Lilac (Code 0005) p. 56

### ✦ Cono 20°

- Platform: Regular/Wide (Code 0066) p. 111

### ✦ Evolution (Internal)

- Implant: Ø 3  
Platform: 3.0 (Code 0090) p. 119
- Implant: Ø 3,6  
Platform: 3.6 (Code 0006) p. 57
- Implant: Ø 4,2  
Platform: 4.2 (Code 0007) p. 58
- Implant: Ø 4,8  
Platform: 4.8 (Code 0091) p. 120
- Implant: Ø 5,4  
Platform: 5.4 (Code 0092) p. 121

### ✦ Uni Abutment

- Platform: Universal (Code 0008) p. 59

## AVINENT

### ✦ HE/EC

Implant: Ø 3,3/3,8/4/4,2/4,8//4,5/5  
Platform: 4,1 (Code 0024) p. 75

Implant: Ø 4,8  
Platform: 5,1 (Code 0061) p. 107

### ✦ HI/IC

Implant: Ø 3,1//3,5/4  
Platform: 3,5 (Code 0040) p. 89

Implant: Ø 3,3/3,8/4/4,2/4,8//4,5/5  
Platform: 4,1 (Code 0040) p. 89

### ✦ Transepitelial

Platform: Regular (Code 0025) p. 76

## BEGO

### ✦ RS/RXS

Implant: Ø 3,0  
Platform: 3,0 (Code 0049) p.98

### ✦ S/RI/RS/RXS

Implant: Ø 3,25/3,75  
Platform: 3,67 (Code 0050) p. 99

Implant: Ø 4,1  
Platform: 4,1 (Code 0051) p. 100

Implant: Ø 4,5  
Platform: 4,5 (Code 0052) p. 101

Implant: Ø 5,5  
Platform: 5,5 (Code 0081) p. 115

## BIOCONCEPT

### ✦ BC Tissue Level Standard

Implant: Ø 3,3/4,1/4,8  
Platform: Regular (Code 0037) p. 86

### ✦ BC Tissue Level Standard Plus

Implant: Ø 4,8  
Platform: Regular (Code 0037) p. 86

### ✦ BC Tissue Level Tapered Effect

Implant: Ø 4,8  
Platform: Regular (Code 0037) p. 86

### ✦ BC Bone Level

Implant: Ø 3,3  
Platform: Narrow (Code 0033) p. 84

Implant: Ø 4,1/4,8  
Platform: Regular (Code 0035) p. 85

### ✦ BV Tapered Bone Level

Implant: Ø 3,5  
Platform: Narrow (Code 0029) p. 80

Implant: Ø 4/4,5/5  
Platform: Regular (Code 0030) p. 81

## BIOGENESIS

### ✦ 3icon

Implant: Ø 3,3  
Platform: Mini (Pink) (Code 0023) p. 74

Implant: Ø 3,75/4/4,3/4,5  
Platform: Regular (Blue) (Code 0024) p. 75

Implant: Ø 5/5,5  
Platform: Wide (Yellow) (Code 0058) p. 104

### ✦ Aticon

Implant: Ø 3,5/4/4,5/5  
Platform: Blue (Code 0005) p. 56

### ✦ Aticon (Cone 20°)

Platform: Regular/Wide (Code 0066) p. 111

## ✦ Iticon

Implant: Ø 3,5/4,1/4,8  
Platform: 4,8 (Code 0037) p. 86

## BIOHORIZONS

### ✦ Tapered Internal

Implant: Ø 3/3,4  
Platform: 3 (Grey) (Code 0102) p. 124

Implant: Ø 3,8  
Platform: 3,5 (Yellow) (Code 0040) p. 89

Implant: Ø 4,6  
Platform: 4,5 (Green) (Code 0041) p. 91

Implant: Ø 5,8  
Platform: 5,7 (Blue) (Code 0080) p. 114

### ✦ Internal

Implant: Ø 3,5/4  
Platform: 3,5 (Yellow) (Code 0040) p. 89

Implant: Ø 4/5  
Platform: 4,5 (Green) (Code 0041) p. 91

Implant: Ø 5/6  
Platform: 5,7 (Blue) (Code 0080) p. 114

### ✦ Multi Unit

Platform: Universal (Code 0025) p. 76

## BIOMET 3i

### ✦ Osseotite

Implant: Ø 3,25  
Platform: 3,4 (Code 0003) p. 54

Implant: Ø 3,75/4  
Platform: 4,1 (Code 0024) p. 75

Implant: Ø 5  
Platform: 5 (Code 0058) p. 104

## ✦ Certain

Implant: Ø 3,25/4  
Platform: 3,4 (Code 0001) p. 52

Implant: Ø 4/5  
Platform: 4,1 (Code 0002) p. 53

Implant: Ø 5  
Platform: 5 (Code 0057) p. 103

### ✦ Low Profile

Platform: Universal (Code 0025) p. 76

## BIOLOK

### ✦ External Hexagon

Implant: Ø 3,45  
Platform: 3,45 (Code 0003) p. 54

## BIONER

### ✦ Ikelt / Bikelt

Implant: Ø 3,3/3,75/4  
Platform: 4,1 (Code 0024) p. 75

### ✦ Ikelt

Implant: Ø 5  
Platform: 5 (Code 0058) p. 104

### ✦ Hikelt

Implant: Ø 3,8  
Platform: 3,95 (Code 0040) p. 89

Implant: Ø 4,7  
Platform: 4,9 (Code 0041) p. 91

### ✦ TopDM

Implant: Ø 3,5  
Platform: 3,5 (Code 0021) p. 72

Implant: Ø 4  
Platform: 4 (Code 0021) p. 72

Implant: Ø 5  
Platform: 5 (Code 0021) p. 72

## ✦ Transepitelial A-5M

Platform: Regular (Code 0025) p. 76

## BIOTEC

### ✦ SPR/CIM

Implant: Ø 3,3  
Platform: 3,3 (Code 0040) p. 89

Implant: Ø 3,75  
Platform: 3,75 (Code 0040) p. 89

### ✦ SPR/SPTT/CIM

Implant: Ø 4,2  
Platform: 4,2 (Code 0040) p. 89

Implant: Ø 5  
Platform: 5 (Code 0040) p. 89

## BIOTECH

### ✦ Kontakt

Implant: Ø 3  
Platform: Yellow Narrow (Code 0164) p. 146

Implant: Ø 3,6/4,2/4,8/5,4  
Platform: Regular (Code 0165) p. 147

## BREDDENT MEDICAL

### ✦ Narrow Sky

Implant: Ø 3,5  
Platform: NP 3,5 (Code 0110) p. 126

### ✦ Blue Sky

Implant: Ø 3,5/4/4,5/5,5  
Platform: 4 (Code 0111) p. 127

### ✦ Blue Sky Classic

Implant: Ø 3,5/4/4,5  
Platform: 4 (Code 0111) p. 127

## BTI

### ✦ External Connection Tiny

Implant: Ø 2,5/3/3,3/3,5/3,75  
Platform: Tiny 3,5 (Code 0009) p. 60

### ✦ ExternalConnection

Implant: Ø 3,75/4/4,5/5  
Platform: Universal 4,1 (Code 0024) p. 75

Implant: Ø 4,5/5/5,5  
Platform: Ancha 5,5 (Code 0060) p. 106

### ✦ InternalConnection

Implant: Ø 3,3/3,5/3,75/4/4,25/4,5/5/5,5  
Platform: Universal 4,1 (Code 0010) p. 61

Implant: Ø 5/5,5/6/6,25  
Platform: Ancha 5,5 (Code 0059) p. 105

### ✦ Multi-IM

Platform Universal 4,1 (Code 0151) p. 140

## BTK

### ✦ Klassic / Konic

Implant: Ø 3,25  
Platform: 3,4 EN (Code 0003) p. 54

Implant: Ø 3,25PL/3,75/4  
Platform: 4,1 ER (Code 0024) p. 75

Implant: Ø 3,25/4  
Platform: 3,5 IR (Code 0040) p. 89

## B&W

### ✦ External Hexagon

Implant: Ø 3,75/4  
Platform: 4,1 (Code 0024) p. 75

Implant: Ø 5  
Platform: 5 (Code 0058) p. 104

### ✦ Internal Hexagon CIH

Implant: Ø 3,3/4  
Platform: 4 (Code 0040) p. 89

## CAMLOG

### ★ Camlog Screw-Line

Implant: Ø 3,8  
Platform: 3,8 (Code 0011) p. 62

Implant: Ø 4,3  
Platform: 4,3 (Code 0012) p. 63

### ★ Conelog Screw-Line

Implant: Ø 3,8  
Platform: 3,8 (Code 0120) p. 128

Implant: Ø 4,3  
Platform: 4,3 (Code 0121) p. 129

## CONEXÃO SISTEMA DE PRÓTESE

### ★ Flash

Implant: Ø 3,5/4,3/5  
Platform: Universal (Code 0021) p. 72

### ★ Torq

Implant: Ø 3,5/3,75/4  
Platform: Universal (Code 0021) p. 72

### ★ Expand

Implant: Ø 3,75/4/5  
Platform: Universal (Code 0021) p. 72

## CORTEX

### ★ Dynamix

Implant: Ø 3,3/3,8/4,2/5/6  
Platform: 3,75 (Code 0040) p. 89

### ★ Classix

Implant: Ø 3,3/3,8/4,2/5/6  
Platform: 3,75 (Code 0040) p. 89

## ★ Saturn

Implant: Ø 3,8/4,2  
Platform: 3,5 (Code 0040) p. 89

### ★ Conical Platform:

Implant: Ø 3  
Platform: NP (Code 0109) p. 125

Implant: Ø 3,3/3,8/4,2  
Platform: RP (Code 0004) p. 55

Implant: Ø 5/6  
Platform: WP (Code 0005) p. 56

### ★ Magix

Implant: Ø 3,3/3,8/4,2  
Platform: RP (Code 0004) p. 55

### ★ Multi Unit

Platform Universal (Code 0025) p. 76

## DENTAL TECH

### ★ Implogic

Implant: Ø 4,5  
Platform: 4,5 (Blue) (Code 0041) p. 91

## DENTAURUM

### ★ Tiologic

Implant: Ø 3,3  
Platform: Small (Code 0130) p. 134

Implant: Ø 3,7/4,2  
Platform: Medium (Code 0131) p. 135

Implant: Ø 4,8/5,5  
Platform: Large (Code 0132) p. 136

## DENTIS

### ★ s-Clean

Implant: Ø 3,7  
Platform: Mini (Code 0030) p. 81

Implant: Ø 4,1/4,3  
Platform: Regular (Code 0030) p. 81

Implant: Ø 4,8  
Platform: Wide (Code 0030) p. 81

## DENTIUM

### ★ SimpleLine II

Implant: Ø 3,8/4,3  
Platform: 4,8 (Code 0074) p. 112

Implant: Ø 3,8/4,3  
Platform: 4,8 (Code 0037) p. 86

Implant: Ø 4,3/4,8  
Platform: 6,5 (Code 0096) p. 122

### ★ SuperLine and Implantium

Implant: Ø 3,4  
Platform: 3,6 (Code 0030) p. 81

Implant: Ø 3,8  
Platform: 4 (Code 0030) p. 81

Implant: Ø 4,3  
Platform: 4,5 (Code 0030) p. 81

Implant: Ø 4,8  
Platform: 5 (Code 0030) p. 81

Implant: Ø 4,8  
Platform: 6 (Code 0030) p. 81

## DIO IMPLANTS

### ★ SM System

Implant: Ø 4,5/5/5,3  
Platform: Regular/Wide (Code 0013) p. 64

### ★ UF II Narrow

Implant: Ø 3/3,3  
Platform: Narrow (Code 0014) p. 65

## ★ UF II

Implant: Ø 3,8/4,4/5/5/5,5  
Platform: Regular (Code 0030) p. 81

### ★ External

Implant: Ø 3,3/3,8  
Platform: Narrow 3,5 (Code 0023) p. 74

Implant: Ø 3,75/4/4,5  
Platform: Regular 4,1 (Code 0024) p. 75

Implant: Ø 5/5,3/5,5/6  
Platform: Wide 5,1 (Code 0061) p. 107

## DSP BIOMEDICAL

### ★ External Hexagon

Implant: Ø 3,75/4/5//3,5/3,8/4,3  
Platform: 4,1 (Code 0024) p. 75

## EASY IMPLANT

### ★ Master C

Implant: Ø 3,5  
Platform: 3,5 (Ocean) (Code 0004) p. 55

Implant: Ø 4  
Platform: 4 (Ocean) (Code 0004) p. 55

Implant: Ø 4,5  
Platform: 4,5 (Lilas) (Code 0030) p. 81

Implant: Ø 5  
Platform: 5 (Lilas) (Code 0030) p. 81

### ★ Master S

Implant: Ø 3,3  
Platform: 3,3 (Ocean) (Code 0004) p. 55

Implant: Ø 3,75  
Platform: 3,75 (Lilas) (Code 0030) p. 81

Implant: Ø 4,25  
Platform: 4,25 (Lilas) (Code 0030) p. 81

Implant: Ø 4,75  
Platform: 4,75 (Lilas) (Code 0030) p. 81

## ★ Master L

Implant: Ø 3,3  
Platform: 3,3 (Lilas) (Code 0030) p. 81

Implant: Ø 3,75  
Platform: 3,75 (Lilas) (Code 0030) p. 81

Implant: Ø 4,25  
Platform: 4,25 (Lilas) (Code 0030) p. 81

Implant: Ø 4,75  
Platform: 4,75 (Lilas) (Code 0030) p. 81

### ★ Multi Unit Conical Abutment

Platform Universal (Code 0025) p. 76

## ECKERMANN

### ★ Hexagon

Implant: Ø 3/3,5/4/4,5/5  
Platform: 4,1 (Code 0024) p. 75

## ELITE MEDICA

### ★ External Connection

Implant: Ø 3,75  
Platform: Narrow (Code 0023) p. 74

Implant: Ø 4  
Platform: Regular (Code 0024) p. 75

Implant: Ø 5  
Platform: Wide (Code 0061) p. 107

## EUROTEKNIKA

### ★ Naturactis

Implant: Ø 3,5  
Platform: 3,4 (Code 0004) p. 55

Implant: Ø 4  
Platform: 3,8 (Code 0004) p. 55

Implant: Ø 4,5  
Platform: 4,3 (Code 0004) p. 55

Implant: Ø 5  
Platform: 4,8 (Code 0004) p. 55

## ★ Uneva

Implant: Ø 3,6  
Platform: 4,1 (Code 0024) p. 75

Implant: Ø 4,1  
Platform: 4,1 (Code 0024) p. 75

### ★ Uneva (Platform: Switching)

Implant: Ø 4,8  
Platform: 4,1 (Code 0024) p. 75

Implant: Ø 6  
Platform: 4,1 (Code 0024) p. 75

### ★ Natea

Implant: Ø 3,6/4,1/4,8  
Platform: Narrow (Code 0004) p. 55

Implant: Ø 3,6/4,1/4,8  
Platform: Regular (Code 0004) p. 55

Implant: Ø 6  
Platform: Wide (Code 0004) p. 55

### ★ Aesthetica

Implant: Ø 4,1  
Platform: 4,8 (Code 0074) p. 112

Implant: Ø 4,1  
Platform: 4,8 (Code 0037) p. 86

Implant: Ø 4,8  
Platform: 6,5 (Code 0096) p. 122

### ★ Naturall

Implant: Ø 3,5  
Platform: Narrow (Code 0004) p. 55

Implant: Ø 4/4,5  
Platform: Regular (Code 0004) p. 55

Implant: Ø 5  
Platform: Wide (Code 0004) p. 55

### ★ Multi Unit Tetra

Platform Universal (Code 0025) p. 76

## GALIMPLANT

### External Connection

Implant: Ø 3,5/4  
Platform: 4 (Code 0024) p. 75

### Internal Connection

Implant: Ø 3,5  
Platform: 3,5 (Code 0004) p. 55

Implant: Ø 4  
Platform: 4 (Code 0004) p. 55

Implant: Ø 5  
Platform: 5 (Code 0004) p. 55

### AbutmentMulti-Position

Platform: Universal (Code 0025) p. 76

## GMI (ILERIMPLANT)

### Phoenix

Implant: Ø 3,3/3,75/4  
Platform: Standard 4,1 (Code 0024) p. 75

Implant: Ø 5  
Platform: Wide 5,1 (Code 0061) p. 107

### Frontier

Implant: Ø 3,3/3,75/4,25  
Platform: RP 3,3 (Code 0040b) p. 90

Implant: Ø 4,75/5,75  
Platform: WP 4,3 (Code 0041b) p. 92

### Universal

Platform: PS-RP 4,8 (Code 0025) p. 76

## GT MEDICAL

### Best Fit Internal Octagon

Implant: Ø 3,7/4,3/4,8  
Platform: Regular (Code 0074) p. 112

Implant: Ø 3,7/4,3/4,8  
Platform: Regular (Code 0037) p. 86

### Best Fit Internal Hexagon

Implant: Ø 3,7/4,1/4,3/4,8  
Platform: Wide (Code 0005) p. 56

### Best Fit External Hexagon

Implant: Ø 3,5  
Platform: Narrow (Code 0023) p. 74

Implant: Ø 4,1  
Platform: Regular (Code 0024) p. 75

Implant: Ø 5,1  
Platform: Wide (Code 0061) p. 107

## HAHN IMPLANT (GLIDEWELL)

### Hahn Tapered Implant

Implant: Ø 3,5/4,3  
Platform: 3,5/4,3 (Code 0021) p. 72

Implant: Ø 5  
Platform: 5 (Code 0022) p. 73

Implant: Ø 7  
Platform: 7 (Code 0124) p. 130

### Multi Unit Abutment system

Platform: Universal (Code 0025) p. 76

## HI-TEC

### Tapered Self Thread

Implant: Ø 3,3/3,75  
Platform: 3,5 (Code 0040) p. 89

Implant: Ø 4,2/5  
Platform: 4,5 (Code 0041) p. 91

### Logic Plus

Implant: Ø 3,5  
Platform: 3,7 (Code 0040) p. 89

Implant: Ø 4,3  
Platform: 3,9 (Code 0040) p. 89

## IDO IMPLANTS

### Ido Implant

Implant: Ø 3,8/4,4/5/5/5/6/7  
Platform: Universal (Code 0030) p. 81

## IHDE DENTAL (IMBIODENT)

### Bone Level Plus

Implant: Ø 3,3  
Platform: 3,3 (Code 0033) p. 84

Implant: Ø 4,1  
Platform: 4,1 (Code 0035) p. 85

Implant: Ø 4,8  
Platform: 4,8 (Code 0035) p. 85

## IMPLANT DIRECT

### RePlus / Replant / Reactive

Implant: Ø 3,5/3,7/4,2  
Platform: 3,5 (Code 0026) p. 77

Implant: Ø 4,3/4,7  
Platform: 4,3 (Code 0027) p. 78

Implant: Ø 5/5,7  
Platform: 5 (Code 0028) p. 79

### Legacy

Implant: Ø 3,7/4,2  
Platform: 3,5 (Code 0040) p. 89

Implant: Ø 4,7/5,2  
Platform: 4,5 (Code 0041) p. 91

### Swishplant / Swishplus

Implant: Ø 4,1/4,8  
Platform: 4,8 (Code 0074) p. 112

Implant: Ø 4,1/4,8  
Platform: 4,8 (Code 0037) p. 86

### SwishActive

Implant: Ø 3,3  
Platform: 3 (Code 0021) p. 72

Implant: Ø 4,1/4,8  
Platform: 3,4 (Code 0022) p. 73

### Interactive

Implant: Ø 3,2/3,7  
Platform: 3 (Code 0021) p. 72

Implant: Ø 4,3/5  
Platform: 3,4 (Code 0022) p. 73

## IMPLANT GENESIS

### Aktiv System

Implant: Ø 3,5/3,75/4,2/5  
Platform: Standard (Code 0040) p. 89

## INTRA-LOCK

### Unihex

Implant: Ø 4  
Platform: Regular (Code 0024) p. 75

Implant: Ø 4,75  
Platform: Wide (Code 0024) p. 75

### IntraHex

Implant: Ø 3,75/4  
Platform: 3,5 (Code 0040) p. 89

Implant: Ø 4,75  
Platform: 4,5 (Code 0041) p. 91

## JDENTALCARE

### JDEvolution/JDEvolution Plus

Implant: Ø 3,7  
Platform: 3,7 (Code 0040) p. 89

Implant: Ø 4,3/5  
Platform: 4 (Code 0040) p. 89

Implant: Ø 6  
Platform: 5 (Code 0040) p. 89

### JD ICON

Implant: Ø 3,9  
Platform: 3,9 (Code 0022) p. 73

Implant: Ø 4,3  
Platform: 4 (Code 0022) p. 73

Implant: Ø 5  
Platform: 4,7 (Code 0022) p. 73

## KEYSTONE

### Restore

Implant: Ø 3,75/4  
Platform: RD 4,1 (Code 0024) p. 75

### Internal TiLobe PrimaConnex

Implant: Ø 3,3/3,5  
Platform: 3,5 (Code 0044) p. 93

Implant: Ø 4/4,1  
Platform: 4,1 (Code 0045) p. 94

Implant: Ø 5  
Platform: 5 (Code 0046) p. 95

## KLOCKNER

### Essential Cone

Implant: Ø 3,5/4/4,5  
Platform: 4,5 (Code 0054) p. 102

### KL

Implant: Ø 3,5  
Platform: Narrow (Code 0023) p. 74

Implant: Ø 4,1  
Platform: Regular (Code 0024) p. 75

Implant: Ø 5,1  
Platform: Wide (Code 0061) p. 107

### Vega

Implant: Ø 3,5  
Platform: NV (Code 0082) p. 116

Implant: Ø 4/4,5  
Platform: RV (Code 0083) p. 117

## LASAK

### Bioniq

Implant: Ø 2,9  
Platform: QN (Yellow) (Code 0166) p. 148

Implant: Ø 3,5/4/5  
Platform: QR (Blue) (Code 0167) p. 149

### Multi Unit

Implant: Ø  
Platform: Universal (Code 0168) p. 150

## LEADER

### Tixos Internal Hex

Implant: Ø 3,3  
Platform: 3,5 (Code 0040) p. 89

Implant: Ø 3,75  
Platform: 4 (Code 0040) p. 89

## ✦ Tixos External Hex

Implant: Ø 3,3/3,75  
Platform: 4,1 (Code 0024) p. 75

Implant: Ø 5  
Platform: 5 (Code 0058) p. 104

## MEDENTIS

### ✦ ICX-Templant

Implant: Ø 3,75  
Platform: 3,75 (Code 0125) p. 131

Implant: Ø 4,1  
Platform: 4,1 (Code 0125) p. 131

Implant: Ø 4,8  
Platform: 4,8 (Code 0125) p. 131

## MEGAGEN

### ✦ AnyRidge

Implant: Ø 3,5  
Platform: Small (Code 0015) p. 66

Implant: Ø 4/4,5  
Platform: Regular (Code 0015) p. 66

Implant: Ø 5/5,5  
Platform: Wide (Code 0015) p. 66

### ✦ AnyOne Internal

Implant: Ø 3,5/4/4,5/5/6/7  
Platform: General (Code 0030) p. 81

### ✦ AnyOne External

Implant: Ø 3,5  
Platform: Small 3,5 (Code 0023) p. 74

Implant: Ø 4  
Platform: Regular 4,1 (Code 0024) p. 75

Implant: Ø 4,5  
Platform: Regular 4,5 (Code 0024) p. 75

Implant: Ø 5  
Platform: Wide 5 (Code 0058) p. 104

Implant: Ø 6  
Platform: SuperWide 5,5 (Code 0058) p. 104

## ✦ Cone Abutment

Implant: Ø Universal  
Platform: 3,8 (Code 0128) p. 132

Implant: Ø Universal  
Platform: 4,8 (Code 0074) p. 112

### ✦ Mini Narrow Ridge

Implant: Ø 3/3,4  
Platform: Mini (Code 0014) p. 65

### ✦ Multi Unit N Type

Platform: Universal (Code 0025) p. 76

## MICRODENT

### ✦ Universal

Implant: Ø 2,8/3,25  
Platform: 3,5 (Code 0003) p. 54

Implant: Ø 3,3/3,5/3,75/4  
Platform: 4,1 (Code 0024) p. 75

Implant: Ø 4,2/5  
Platform: 5,1 (Code 0058) p. 104

### ✦ System

Implant: Ø 2,8/3,25  
Platform: 3,5 (Code 0003) p. 54

### ✦ Ektos

Implant: Ø 3,7/4,2  
Platform: 3,5 (Code 0040b) p. 92

## MIS

### ✦ Lance

Implant: Ø 3,75/4,2  
Platform: Standard (Code 0024) p. 75

Implant: Ø 5  
Platform: Wide (Code 0058) p. 104

### ✦ Multi Unit

Platform: General (Code 0020) p. 71

## ✦ Seven

Implant: Ø 3,3  
Platform: Narrow (Code 0019) p. 70

Implant: Ø 3,75/4,2  
Platform: Standard (Code 0040) p. 89

Implant: Ø 5/6  
Platform: Wide (Code 0041) p. 91

### ✦ M4

Implant: Ø 3,3  
Platform: Narrow (Code 0019) p. 70

Implant: Ø 3,75/4,2  
Platform: Standard (Code 0040) p. 89

Implant: Ø 5/6  
Platform: Wide (Code 0041) p. 91

### ✦ C1

Implant: Ø 3,3  
Platform: Narrow (Code 0016) p. 67

Implant: Ø 3,75/4,2  
Platform: Standard (Code 0017) p. 68

Implant: Ø 5  
Platform: Wide (Code 0018) p. 69

### ✦ V3

Implant: Ø 3,9/4,3/5  
Platform: Standard (Code 0017) p. 68

## MOZO-GRAU

### ✦ MG Osseous

Implant: Ø 3,3  
Platform: 3,4 Mini (Code 0003) p. 54

Implant: Ø 3,4/3,75/4,25  
Platform: 4,1 Standard (Code 0024) p. 75

Implant: Ø 5  
Platform: 5 Maxi (Code 0061) p. 107

## ✦ MG Inhex

Implant: Ø 3,3  
Platform: 2,3 Mini (Code 0109) p. 125

Implant: Ø 3,75/4,25  
Platform: 2,8 Standard (Code 0004) p. 55

Implant: Ø 5  
Platform: 3,8 Maxi (Code 0005) p. 56

## MPI

### ✦ External Connection HE Privilege

Implant: Ø 3,3  
Platform: 3,5 (Code 0009) p. 60

Implant: Ø 3,3/4  
Platform: 4,1 (Code 0024) p. 75

Implant: Ø 5  
Platform: 5 (Code 0058) p. 104

### ✦ Privilege CM

Implant: Ø 3,5/4  
Platform: Regular (Code 0004) p. 55

Implant: Ø 5  
Platform: Wide (Code 0005) p. 56

### ✦ Excellence CM

Implant: Ø 3,5/4  
Platform: Regular (Code 0004) p. 55

Implant: Ø 5  
Platform: Wide (Code 0005) p. 56

## NEOBIO TECH

### ✦ EB External System

Implant: Ø 3,5  
Platform: Narrow (Code 0023) p. 74

### ✦ IS Implant: System

Implant: Ø 4  
Platform: Regular 4 (Code 0030) p. 81

Implant: Ø 4,5  
Platform: Regular 4,5 (Code 0030) p. 81

Implant: Ø 5  
Platform: Wide 5 (Code 0030) p. 81

Platform: 4,8 (Code 0025) p. 76

## NEODENT

### ✦ Helix GM/Drive GM/Titamax GM

Implant: Ø 3,5/3,75/4/4,3/5/6  
Platform: Regular (Code 0186) p. 152

### ✦ Smart HE

Implant: Ø 3,75/4  
Platform: 4,1 (Code 0024) p. 75

### ✦ Mini Pilar CM

Platform: Universal (Code 0025) p. 76

## NEOSS

### ✦ ProActive Straight/Tapered

Implant: Ø 3,5 Green  
Platform: ProActive (Code 0047) p. 96

Implant: Ø 4 Yellow  
Platform: ProActive (Code 0047) p. 96

Implant: Ø 4,5 Blue  
Platform: ProActive (Code 0048) p. 97

Implant: Ø 5 Peach  
Platform: ProActive (Code 0048) p. 97

Implant: Ø 5,5 Lilac  
Platform: ProActive (Code 0048) p. 97

## NOBEL BIOCARE

### ✦ Branemark

Implant: Ø 3,3  
Platform: Narrow (Code 0023) p. 74

Implant: Ø 3,75/4  
Platform: Regular (Code 0024) p. 75

Implant: Ø 5/6  
Platform: Wide (Code 0061) p. 107

## ✦ Multi Unit

Platform: Regular (Code 0025) p. 76

### ✦ Replace

Implant: Ø 3,5  
Platform: Narrow (Code 0026) p. 77

Implant: Ø 4,3  
Platform: Regular (Code 0027) p. 78

Implant: Ø 5  
Platform: Wide (Code 0028) p. 79

Implant: Ø 6  
Platform: Platform: 6 (Code 0129) p. 133

### ✦ Active

Implant: Ø 3  
Platform: Mini 3.0 (Code 0159) p. 141

Implant: Ø 3,5  
Platform: Narrow (Code 0021) p. 72

Implant: Ø 4,3/5  
Platform: Regular (Code 0022) p. 73

Implant: Ø 5,5  
Platform: Wide (Code 0124) p. 130

## NORIS MEDICAL

### ✦ Tuff

Implant: Ø 3,3/3,75/4,2/5/6  
Platform: 3,75 (Code 0040) p. 89

### ✦ Tuff TT

Implant: Ø 3,3/3,75/4,2/5/6  
Platform: 3,75 (Code 0040) p. 89

### ✦ Onix

Implant: Ø 3,3/3,75/4,2/5/6  
Platform: 3,75 (Code 0040) p. 89

### ✦ Cortical

Implant: Ø 4,0/5/6  
Platform: 3,75 (Code 0040) p. 89



✦ PteryCore  
Implant: Ø 4,2  
Platform: 3,75 (Code 0040) p. 89

✦ PteryFit  
Implant: Ø 4,2  
Platform: 3,75 (Code 0040) p. 89

## NORMON

✦ Normoimplant HE  
Implant: Ø 3,25/3,75/4,25/4,75  
Platform: 4,1 (Code 0024) p. 75

✦ Normoimplant HI  
Implant: Ø 3,75/4,25/4,75  
Platform: 3,5 (Code 0040b) p. 90

## NOVA IMPLANTS

✦ PSI/PCI  
Implant: Ø 3,3/3,75/4,2/5/6  
Platform: 3,75 (Code 0040b) p. 90

## OSSTEM IMPLANT

✦ TS  
Implant: Ø 3,5  
Platform: Mini (Code 0029) p. 80  
  
Implant: Ø 4/4,5/5/6/7  
Platform: Regular (Code 0030) p. 81

✦ US  
Implant: Ø 3,3/3,5  
Platform: Mini 3,5 (Code 0023) p. 74  
  
Implant: Ø 3,75/4/4,5  
Platform: Regular 4,1 (Code 0024) p. 75  
  
Implant: Ø 5/5,5  
Platform: Wide 5,1 (Code 0061) p. 107  
  
Implant: Ø 5/5,5  
Platform: Wide PS 5 (Code 0058) p. 104

## OSTEOPLUS

✦ She  
Implant: Ø 3,45  
Platform: 3,45 (Code 0009) p. 60

Implant: Ø 3,75 / 4  
Platform: 4 (Code 0024) p. 75

✦ Shi  
Implant: Ø 3,3 / 3,75 / 4,2  
Platform: 3,5 (Code 0040) p. 89

## PALTOP

✦ Advanced classic  
Implant: Ø 3,75/4,2/5  
Platform: Standard (Code 0040b) p. 90

✦ Advanced +  
Implant: Ø 3,75/4,2/5  
Platform: Standard (Code 0040b) p. 90

✦ Dynamic  
Implant: Ø 3,75/4,2/5  
Platform: Standard (Code 0040b) p. 90

✦ DIVA  
Implant: Ø 3,75/4,2/5  
Platform: Standard (Code 0040b) p. 90

✦ Conical Active  
Implant: Ø 3,75/4,2/5  
Platform: Standard (Code 0029) p. 80

## PHIBO

✦ TSH/BNT Serie 3  
Implant: Ø 3,6  
Platform: 4 (Code 0024) p. 75

✦ TSH/BNT Serie 4  
Implant: Ø 4,2  
Platform: 4 (Code 0024) p. 75

## PROCLINIC

✦ Cylindrical External/Conical External  
Implant: Ø 3,75/4,25//3,5/4  
Platform: 4,1 Estandar (Code 0024) p. 75

Implant: Ø 5  
Platform: 5 Maxi (Code 0058) p. 104

✦ Cylindrical Internal/Conical Internal  
Implant: Ø 3,3/3,75/4,25/5//3,5/4/5  
Platform: 3,5 (Code 0040) p. 89

✦ SP Octa  
Implant: Ø 3,3/4,1/4,8  
Platform: 4,8 (Code 0074) p. 112

Implant: Ø 3,3/4,1/4,8  
Platform: 4,8 (Code 0037) p. 86

Implant: Ø 4,8  
Platform: 6,5 (Code 0096) p. 122

## RADHEX

✦ PHE  
Implant: Ø 3,5  
Platform: 3,5 (Code 0023) p. 74

Implant: Ø 4/4,5/5  
Platform: 4,1 (Code 0024) p. 75

✦ PHI  
Implant: Ø 3,75  
Platform: 3,5 (Code 0040b) p. 90

Implant: Ø 4,5/5  
Platform: 4,5 (Code 0041b) p. 92

## SEWON MEDIX

✦ IH2 SLA SYSTEM  
Implant: Ø 3,5  
Platform: Mini (Code 0029) p. 80

Implant: Ø 3,5/4/4,5/5  
Platform: Regular (Code 0030) p. 81

✦ IH2 RBM SYSTEM  
Implant: Ø 3,5  
Platform: Mini (Code 0029) p. 80

Implant: Ø 3,5/4/4,5/5  
Platform: Regular (Code 0030) p. 81

✦ IH SYSTEM  
Platform: Universal (Code 0025) p. 76

## SGS

✦ P1  
Implant: Ø 3,2/3,75/4,2/5/6  
Platform: 3,75 (Code 0040) p. 89

✦ P7  
Implant: Ø 3,2/3,75/4,2/4,5/5/6  
Platform: 3,75 (Code 0040) p. 89

## SIGNO VINCES

✦ Duo  
Implant: Ø 4,6  
Platform: 4,1 (Code 0024) p. 75

✦ Inttegra  
Implant: Ø 3,75/4  
Platform: 4,1 (Code 0024) p. 75

✦ Compact  
Implant: Ø 4,5  
Platform: CM3,8 (Code 0004) p. 55

✦ Duocon  
Implant: Ø 3,8  
Platform: CM3,8 (Code 0004) p. 55

Implant: Ø 4,6/5,5  
Platform: CM4,6 (Code 0005) p. 56

✦ Infra  
Implant: Ø 3,3/3,8/4,6  
Platform: CM (Code 0004) p. 55

## SOUTHERN IMPLANTS

✦ Tri-Nex  
Implant: Ø 3,5  
Platform: 3,5 (Code 0026) p. 77

Implant: Ø 4,3  
Platform: 4,3 (Code 0027) p. 78

Implant: Ø 5  
Platform: 5 (Code 0028) p. 79

✦ IT Connection  
Implant: Ø 3,3/4/4,1/4,9/5  
Platform: 4,8 (Code 0037) p. 86

Implant: Ø 4,9/5/6  
Platform: 6,5 (Code 0096) p. 122

✦ External Hex  
Implant: Ø 3,25  
Platform: 3,4 (Code 0003) p. 54

Implant: Ø 3,75/4  
Platform: 4,1 (Code 0024) p. 75

Implant: Ø 4,7/5  
Platform: 5 (Code 0058) p. 104

Implant: Ø 5,7/6  
Platform: 6 (Code 0058) p. 104

✦ Deep Conical  
Implant: Ø 3  
Platform: 2,45 (Code 0109) p. 125

Implant: Ø 3,5/4  
Platform: 2,95/3,1 (Code 0004) p. 55

Implant: Ø 5  
Platform: 4,1 (Code 0005) p. 56

✦ Internal Hex  
Implant: Ø 3,75/4,2/5  
Platform: Universal (Code 0040) p. 89

✦ Compact Conical  
Platform: 4,8 (Code 0025) p. 76

## STERNGOLD

✦ STERN EX  
Implant: Ø 3,75/4/5  
Platform: 4,1 (Code 0024) p. 75

## STRAUMANN

✦ Tissue Level  
Implant: Ø 3,3/4,1/4,8  
Platform: Regular 4,8 (Code 0037) p. 86

Implant: Ø 4,8  
Platform: Wide 6,5 (Code 0096) p. 122

✦ Synocta  
Implant: Ø 4,8  
Platform: Regular 4,8 (Code 0074) p. 112

Implant: Ø 6,5  
Platform: Wide 6,5 (Code 0137) p. 138

## ✦ Bone Level

Implant: Ø 3,3  
Platform: NC- 3,3 (Code 0033) p. 84

Implant: Ø 4,1  
Platform: RC-4,1 (Code 0035) p. 85

Implant: Ø 4,8  
Platform: RC-4,8 (Code 0035) p. 85

## ✦ Tissue Level NNC

Implant: Ø 3,3  
Platform: 3,5 (Code 0160) p. 142

## ✦ Screw-Retained

Implant: Ø Universal  
Platform: NC/RC (Code 0101) p. 123

## SWEDEN&MARTINA

### ✦ Outlink2

Implant: Ø 3,3  
Platform: 3,3 (Code 0063) p. 108

Implant: Ø 3,75/4,1  
Platform: 4,1 (Code 0064) p. 109

### ✦ Shelta

Implant: Ø 3,8  
Platform: 3,8 (Code 0032) p. 83

Implant: Ø 4,25  
Platform: 4,25 (Code 0032) p. 83

Implant: Ø 5  
Platform: 5 (Code 0032) p. 83

### ✦ Premium Kohno

Implant: Ø 3,3  
Platform: 3,3 (Code 0031) p. 82

Implant: Ø 3,8  
Platform: 3,8 (Code 0032) p. 83

Implant: Ø 4,25  
Platform: 4,25 (Code 0065) p. 110

## SYBRON IMPLANT SOLUTIONS

### ✦ Endopore (Innova)

Implant: Ø 4,1  
Platform: 4,1 (Code 0024) p. 75

## TITANIUM-FIX

### ✦ b-fix

Implant: Ø 3,5/4  
Platform: Regular (Code 0004) p. 55

Implant: Ø 4,5/5  
Platform: Larga (Code 0005) p. 56

## TRE-OSS

### ✦ Simple

Implant: Ø 3,3/3,75/5  
Platform: 3,75 Amarillo (Code 0040) p. 89

## TRI DENTAL IMPLANTS

### ✦ TRI-Vent

Implant: Ø 3,75/4,1/4,7  
Platform: 3,5 (Code 0040) p. 89

## TRINON

### ✦ Q2

Implant: Ø 3,5/3,75/4,5  
Platform: 4 (Code 0024) p. 75

### ✦ QK

Implant: Ø 4  
Platform: 4,8 (Code 0074) p. 112

Implant: Ø 4  
Platform: 4,8 (Code 0037) p. 86

## UFIT

### ✦ Gt2

Implant: Ø 3,5  
Platform: Mini (Code 0004) p. 55

Implant: Ø 4/4,5  
Platform: Regular (Code 0005) p. 56

Implant: Ø 5  
Platform: Wide (Code 0005) p. 56

Implant: Ø 5,5/6/6,5/7  
Platform: Ultra-wide (Code 0005) p. 56

### ✦ Nt2

Implant: Ø 3,5  
Platform: Mini (Code 0004) p. 55

Implant: Ø 4/4,5  
Platform: Regular (Code 0005) p. 56

Implant: Ø 5  
Platform: Wide (Code 0005) p. 56

Implant: Ø 5,5/6/6,5/7  
Platform: Ultra-wide (Code 0005) p. 56

## VULKAN IMPLANTS

### ✦ IN-Hex

Implant: Ø 3,3/3,75/4,2/5  
Platform: 3,75 (Code 0040) p. 89

## XIVE

### ✦ Xive

Implant: Ø 3,4  
Platform: 3,4 (Code 0038) p. 87

Implant: Ø 3,8  
Platform: 3,8 (Code 0039) p. 88

Implant: Ø 4,5  
Platform: 4,5 (Code 0085) p. 118

## YES IMPLANT

### ✦ S-SYSTEM

Implant: Ø 3,3/3,5  
Platform: Narrow (Code 0030) p. 81

Implant: Ø 4/4,5  
Platform: Regular (Code 0030) p. 81

Implant: Ø 5/5,5  
Platform: Wide (Code 0030) p. 81

## ZIACOM (OSSEOLIFE)

### ✦ OEX

Implant: Ø 3,75/4,25  
Platform: RP 4,1 (Code 0024) p. 75

## ZIMMER

### ✦ Screw-Vent

Implant: Ø 3,7/4,1  
Platform: 3,5 (Code 0040) p. 89

Implant: Ø 4,7  
Platform: 4,5 (Code 0041) p. 91

Implant: Ø 6  
Platform: 5,7 (Code 0080) p. 114

### ✦ Swiss-Plus

Implant: Ø 3,7/4,1/4,8  
Platform: 4,8 (Code 0074) p. 112

Implant: Ø 3,7/4,1/4,8  
Platform: 4,8 (Code 0037) p. 86

# COMPATIBLE with 0001

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			1,2 mm			mm			mm			mm		
R	31.322.001.01-2	43°	29°	31.322.001.02-2	25°	22°	-	-	-	-	-	-	-	-	-
NR	31.312.001.01-2			31.312.001.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.103.01-2	10	50.312.001.01-2	43.621.410.01-2	34.612.001.01-2	32.212.001.02-2	25°	33.390.754.01-2	3	25°
			43.624.410.01-2				33.490.754.01-2	4	
52.412.103.01-2	12		43.630.410.01-2				33.690.754.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.316.084.01-2	-	43.618.201.01-2	18	40.316.003.01-2	43.601.103.02-2	22.612.001.01-2	30.412.001.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0001	LAB SCANBODY	DAS_C_E_0001
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0001	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0001
	DAS_I_12_0001		DAS_C_I_12_0001

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

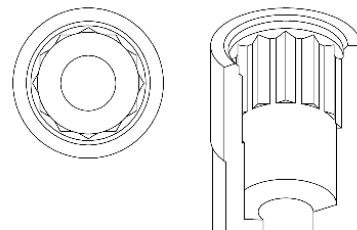

# COMPATIBLE with 0002

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			1,2 mm			mm			mm			mm		
R	31.323.002.01-2	45°	29°	31.323.002.02-2	25°	22°	-	-	-	-	-	-	-	-	-
NR	31.313.002.01-2			31.313.002.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	31.323.002.21-2	25°	20°	10°
NR	-			

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.101.01-2	8	50.313.002.01-2	43.621.410.01-2	34.613.002.01-2	32.213.002.02-2	30°	33.390.805.01-2	3	30°
52.410.101.01-2	10		43.624.410.01-2				33.490.805.01-2	4	
52.412.101.01-2	12		43.630.410.01-2				33.690.805.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.316.084.01-2	-	43.618.201.01-2	18	40.316.003.01-2	43.601.103.02-2	22.613.002.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0002	LAB SCANBODY	DAS_C_E_0002
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_8_0002	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_8_0002
	DAS_I_10_0002		DAS_C_I_10_0002
	DAS_I_12_0002		DAS_C_I_12_0002

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

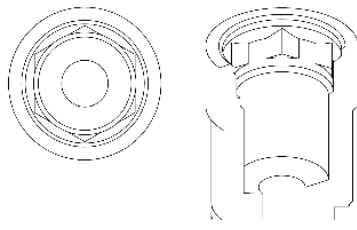

# COMPATIBLE with 0003

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			mm			mm			mm			mm		
R	31.322.003.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.003.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.104.01-2	10	50.312.003.01-2	43.621.410.01-2	34.612.003.01-2	-	-	33.390.716.01-2	3	25°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.104.01-2	12	43.630.410.01-2	33.690.716.01-2	6					

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.320.065.01-2	-	43.618.201.01-2	18	40.320.003.02-2	43.601.103.02-2	22.612.003.01-2	30.412.001.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0003	LAB SCANBODY	DAS_C_E_0003
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0003	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0003
	DAS_I_12_0003		DAS_C_I_12_0003

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

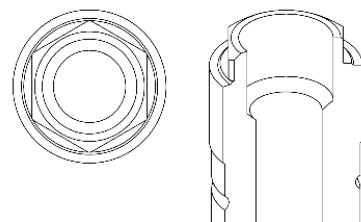

# COMPATIBLE with 0004

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1 mm			2 mm			mm			mm			mm		
R	31.323.004.01-2	45°	29°	31.323.004.02-2	30°	20°	-	-	-	-	-	-	-	-	-
NR	31.313.004.01-2			31.313.004.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	31.323.004.21-2	25°	20°	10°
NR	31.313.004.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.103.01-2	10	50.313.004.01-2	43.621.410.01-2	34.613.004.01-2 (1) 34.613.004.02-2 (2)	32.213.004.02-2	25°	33.390.754.01-2	3	25°
			43.624.410.01-2				33.490.754.01-2	4	
52.412.103.01-2	12	43.630.410.01-2	33.690.754.01-2	6					

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.076.01-2	-	43.618.201.01-2	18	40.316.005.02-2	43.601.105.01-2	22.613.004.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0004	LAB SCANBODY	DAS_C_E_0004
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0004	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0004
	DAS_I_12_0004		DAS_C_I_12_0004

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

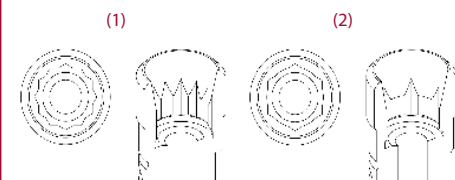



# COMPATIBLE with 0005

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1 mm			2 mm			mm			mm			mm		
R	31.324.005.01-2	38°	23°	31.324.005.02-2	25°	15°	-	-	-	-	-	-	-	-	-
NR	31.314.005.01-2			31.314.005.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	1 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.324.005.21-2	25°	20°	10°
NR	31.314.005.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.102.01-2	10	50.314.005.01-2	43.621.410.01-2	34.614.005.01-2	-	-	33.390.958.01-2	3	30°
			43.624.410.01-2				33.490.958.01-2	4	
52.412.102.01-2	12		43.630.410.01-2				33.690.958.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.320.090.01-2	-	43.618.201.01-2	18	40.320.005.03-2	43.601.105.01-2	22.614.005.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0005	LAB SCANBODY	DAS_C_E_0005
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0005	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0005
	DAS_I_12_0005		DAS_C_I_12_0005

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

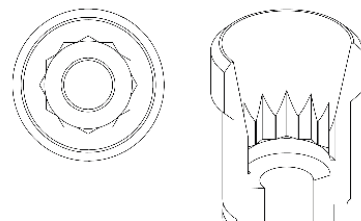

# COMPATIBLE with 0006

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,2 mm			mm			mm			mm			mm		
R	31.322.006.01-2	40°	20°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.006.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.105.01-2	10	50.312.006.01-2	43.621.410.01-2	34.612.006.01-2	32.212.006.02-2	25°	33.330.734.01-2	3	25°
			43.624.410.01-2				33.430.734.01-2	4	
52.412.105.01-2	12		43.630.410.01-2				33.630.734.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.072.01-2	-	43.618.201.01-2	18	40.316.005.01-2	43.601.105.01-2	2.612.006.01-2	30.412.001.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0006	LAB SCANBODY	DAS_C_E_0006
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0006	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0006
	DAS_I_12_0006		DAS_C_I_12_0006

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

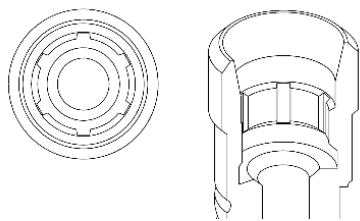

# COMPATIBLE with 0007

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,5 mm			mm			mm			mm			mm		
R	31.323.007.01-2	38°	17°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.007.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	1,5 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.323.007.21-2	25°	20°	10°
NR	31.313.007.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.101.01-2	8	50.313.007.01-2	43.621.410.01-2	34.613.007.01-2	32.213.007.02-2	25°	33.350.775.01-2	3	25°
52.410.101.01-2	10		43.624.410.01-2				33.450.775.01-2	4	
52.412.101.01-2	12		43.630.410.01-2				33.650.775.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.318.074.01-2	-	43.618.201.01-2	18	40.318.005.02-2	43.601.105.01-2	22.613.007.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0007	LAB SCANBODY	DAS_C_E_0007
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0007	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0007
	DAS_I_10_0007		DAS_C_I_10_0007
	DAS_I_12_0007		DAS_C_I_12_0007

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

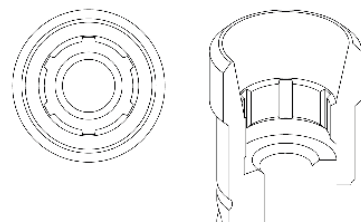

# COMPATIBLE with 0008

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.323.008.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	0,5 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.323.008.21-2	25°	20°	10°
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.113.01-2	8	50.313.008.01-2	43.621.410.01-2	34.613.008.01-2	-	-	33.370.716.01-2	3	30°
-	10		43.624.410.01-2				33.470.716.01-2	4	
-	12		43.630.410.01-2				33.670.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.318.045.01-2	-	43.618.201.01-2	18	40.318.005.01-2	43.601.105.01-2	-	30.412.001.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0008	LAB SCANBODY	DAS_C_E_0008
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0008	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0008

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

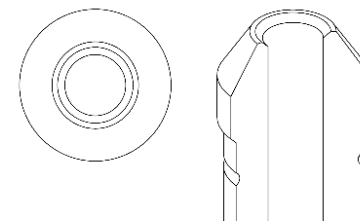

# COMPATIBLE with 0009

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			0,5 mm			1 mm			mm			mm		
R	31.322.009.01-2	45°	25°	31.322.009.02-2	25°	25°	31.322.009.03-2	25°	-	-	-	-	-	-	-
NR	31.312.009.01-2			31.312.009.02-2			31.312.009.03-2			-			-		

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.114.01-2	10	50.312.009.01-2	43.621.410.01-2	34.612.009.01-2	-	-	33.390.716.01-2	3	25°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.114.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.320.051.01-2	-	43.618.201.01-2	18	40.320.003.01-2	43.601.103.02-2	22.612.009.01-2	30.412.001.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0009	LAB SCANBODY	DAS_C_E_0009
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0009	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0009
	DAS_I_12_0009		DAS_C_I_12_0009

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

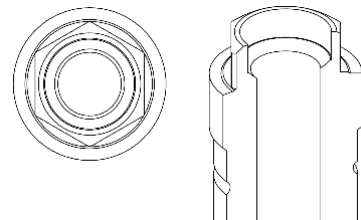

# COMPATIBLE with 0010

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			1 mm			mm			mm			mm		
R	31.323.010.01-2	45°	29°	31.323.010.02-2	30°	28°	-	-	-	-	-	-	-	-	-
NR	31.313.010.01-2			31.313.010.02-2			-			-			-		

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.115.01-2	10	50.313.010.01-2	43.621.410.01-2	34.613.010.01-2	-	-	33.390.716.01-2	3	30°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.115.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.318.065.01-2	-	43.618.201.01-2	18	40.318.003.01-2	43.601.103.02-2	22.613.010.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0010	LAB SCANBODY	DAS_C_E_0010
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0010	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0010
	DAS_I_12_0010		DAS_C_I_12_0010

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

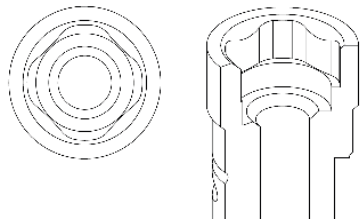



# COMPATIBLE with 0011

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			mm			mm			mm			mm		
R	31.322.011.01-2	30°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.011.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.108.01-2	10	50.312.011.01-2	43.621.410.01-2	34.612.011.01-2	-	-	33.345.804.01-2	3	20°
			43.624.410.01-2				33.445.804.01-2	4	
52.412.108.01-2	12	43.630.410.01-2	33.645.804.01-2	6					

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.094.01-2	-	43.618.201.01-2	18	40.316.005.04-2	43.601.105.01-2	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0011	LAB SCANBODY	DAS_C_E_0011
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0011	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0011
	DAS_I_12_0011		DAS_C_I_12_0011

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

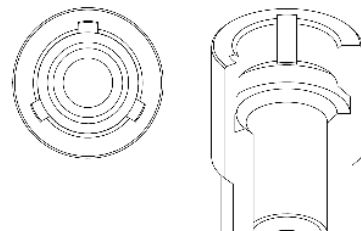

# COMPATIBLE with 0012

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			mm			mm			mm			mm		
R	31.323.012.01-2	33°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.012.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.109.01-2	10	50.313.012.01-2	43.621.410.01-2	34.613.012.01-2	-	-	33.345.804.01-2	3	20°
			43.624.410.01-2				33.445.804.01-2	4	
52.412.109.01-2	12	43.630.410.01-2	33.645.804.01-2	6					

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.094.01-2	-	43.618.201.01-2	18	40.316.005.04-2	43.601.105.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0012	LAB SCANBODY	DAS_C_E_0012
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0012	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0012
	DAS_I_12_0012		DAS_C_I_12_0012

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

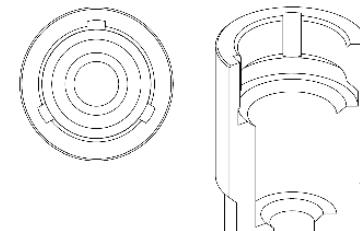

# COMPATIBLE with 0013

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,7 mm			mm			mm			mm			mm		
R	31.323.013.01-2	43°	23°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.013.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$	
-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.320.074.01-2	-	43.618.201.01-2	18	40.320.007.02-2	43.601.107.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0013	LAB SCANBODY	DAS_C_E_0013
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

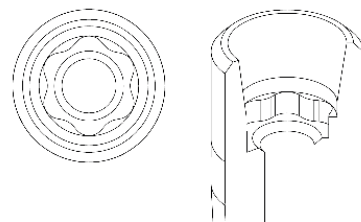

# COMPATIBLE with 0014

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,2 mm			2 mm			3 mm			mm			mm		
R	31.322.014.01-2	41°	23°	31.322.014.02-2	25°	17°	-	20°	25°	-	-	-	-	-	-
NR	31.312.014.01-2			31.312.014.02-2	31.312.014.03-2	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$	
-	-	-	-	-	-	-	-	-	-	
-	-	-	-	-	-	-	-	-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.314.067.01-2	41.314.105.01-2	43.618.201.01-2	18	40.314.003.04-2	43.601.103.02-2	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0014	LAB SCANBODY	DAS_C_E_0014
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

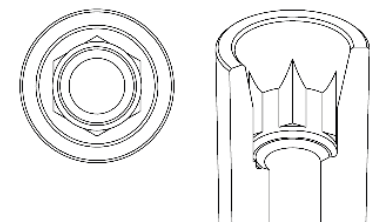

# COMPATIBLE with 0015

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,7 mm			2 mm			mm			mm			mm		
R	31.323.015.01-2	43°	23°	31.323.015.02-2	25°	15°	-	-	-	-	-	-	-	-	-
NR	31.313.015.01-2			31.313.015.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	1,7 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.323.015.21-2	30°	25°	10°
NR	31.313.015.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.104.01-2	10	50.313.015.01-2	43.621.410.01-2	34.613.015.01-2	-	-	33.390.805.01-2	3	25°
			43.624.410.01-2				33.490.805.01-2	4	
52.412.104.01-2	12		43.630.410.01-2				33.690.805.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.318.080.01-2	-	43.618.201.01-2	18	40.318.003.02-2	43.601.103.02-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0015	LAB SCANBODY	DAS_C_E_0015
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0015	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0015
	DAS_I_12_0015		DAS_C_I_12_0015

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

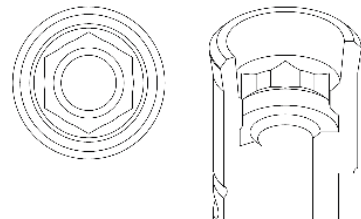

# COMPATIBLE with 0016

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,8 mm			mm			mm			mm			mm		
R	31.322.016.01-2	45°	28°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.016.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.106.01-2	8	50.312.016.01-2	43.621.410.01-2	34.612.016.01-2	-	-	33.360.754.01-2	3	25°
52.410.106.01-2	10		43.624.410.01-2				33.460.754.01-2	4	
52.412.106.01-2	12		43.630.410.01-2				33.660.754.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.071.01-2	-	43.618.201.01-2	18	40.316.005.05-2	43.601.105.01-2	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0016	LAB SCANBODY	DAS_C_E_0016
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0016	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0016
	DAS_I_10_0016		DAS_C_I_10_0016
	DAS_I_12_0016		DAS_C_I_12_0016

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

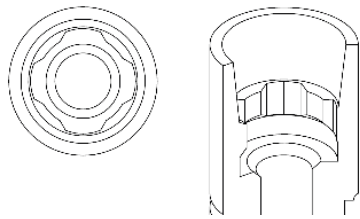



# COMPATIBLE with 0017

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,7 mm			mm			mm			mm			mm		
R	31.323.017.01-2	45°	24°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.017.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.101.01-2	8	50.313.017.01-2	43.621.410.01-2	34.613.017.01-2	-	-	33.360.756.01-2	3	30°
52.410.101.01-2	10		43.624.410.01-2				33.460.756.01-2	4	
52.412.101.01-2	12		43.630.410.01-2				33.660.756.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.317.073.01-2	-	43.618.201.01-2	18	40.317.005.01-2	43.601.105.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0017	LAB SCANBODY	DAS_C_E_0017
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_8_0017	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_8_0017
	DAS_I_10_0017		DAS_C_I_10_0017
	DAS_I_12_0017		DAS_C_I_12_0017

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

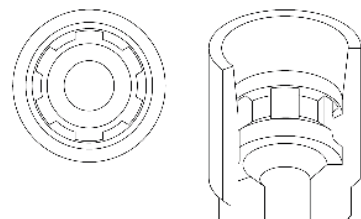

# COMPATIBLE with 0018

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,2 mm			mm			mm			mm			mm		
R	31.324.018.01-2	39°	18°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.018.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.102.01-2	10	50.314.018.01-2	43.621.410.01-2	34.614.018.01-2	-	-	33.360.756.01-2	3	30°
			43.624.410.01-2				33.460.756.01-2	4	
52.412.102.01-2	12		43.630.410.01-2				33.660.756.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.317.073.01-2	-	43.618.201.01-2	18	40.317.005.01-2	43.601.105.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0018	LAB SCANBODY	DAS_C_E_0018
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0018	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0018
	DAS_I_12_0018		DAS_C_I_12_0018

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

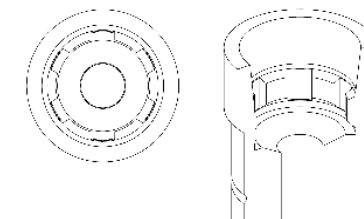

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,8 mm			mm			mm			mm			mm		
R	31.322.019.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.019.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$
52.410.105.01-2	10	50.312.019.01-2	43.621.410.01-2	34.612.019.01-2	-	-
			43.624.410.01-2			
52.412.105.01-2	12		43.630.410.01-2			

DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
33.360.754.01-2	3	25°
33.460.754.01-2	4	
33.660.754.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.071.01-2	-	43.618.201.01-2	18	40.316.005.05-2	43.601.105.01-2	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0019	LAB SCANBODY	DAS_C_E_0019
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0019	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0019
	DAS_I_12_0019		DAS_C_I_12_0019

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

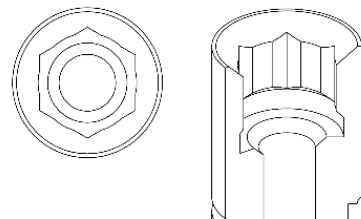

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.323.020.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$
52.408.112.01-2	8	50.313.020.01-2	43.620.411.01-2	34.613.020.01-2	-	-
-	10		43.624.411.01-2			
-	12		43.630.411.01-2			

DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
33.390.716.01-2	3	30°
33.490.716.01-2	4	
33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.044.01-2	-	43.618.201.01-2	18	40.316.005.06-2	43.601.105.01-2	-	-	-	30.413.005.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0020	LAB SCANBODY	DAS_C_E_0020
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_8_0020	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_8_0020

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

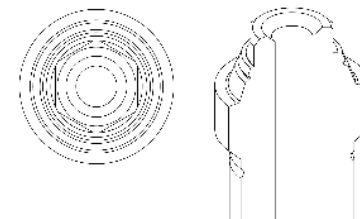

# COMPATIBLE with 0021

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,5 mm			2 mm			mm			mm			mm		
R	31.322.021.01-2	43°	24°	31.322.021.02-2	25°	20°	-	-	-	-	-	-	-	-	-
NR	31.312.021.01-2			31.312.021.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	1,5 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.322.021.21-2	25°	20°	10°
NR	31.312.021.21-2			

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.103.01-2	10	50.312.021.01-2	43.621.410.01-2	34.612.021.01-2	32.212.021.02-2	25°	33.335.754.01-2	3	25°
			43.624.410.01-2				33.435.754.01-2	4	
52.412.103.01-2	12		43.630.410.01-2				33.635.754.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP				
41.316.073.01-2	-	43.618.201.01-2	18	40.316.008.02-2	43.601.108.01-2	22.612.021.01-2	30.412.001.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0021	LAB SCANBODY	DAS_C_E_0021
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0021	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0021
	DAS_I_12_0021		DAS_C_I_12_0021

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

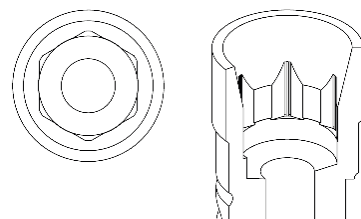

# COMPATIBLE with 0022

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,3 mm			2 mm			mm			mm			mm		
R	31.323.022.01-2	40°	19°	31.323.022.02-2	25°	14°	-	-	-	-	-	-	-	-	-
NR	31.313.022.01-2			31.313.022.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	1,3 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.323.022.21-2	30°	25°	10°
NR	31.313.022.21-2			

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.101.01-2	8	50.313.022.01-2	43.621.410.01-2	34.613.022.01-2	32.213.022.02-2	30°	33.335.758.01-2	3	30°
52.410.101.01-2	10		43.624.410.01-2				33.435.758.01-2	4	
52.412.101.01-2	12		43.630.410.01-2				33.635.758.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP				
41.320.075.01-2	-	43.618.201.01-2	18	40.320.008.02-2	43.601.108.01-2	22.613.022.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0022	LAB SCANBODY	DAS_C_E_0022
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_8_0022	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_8_0022
	DAS_I_10_0022		DAS_C_I_10_0022
	DAS_I_12_0022		DAS_C_I_12_0022

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

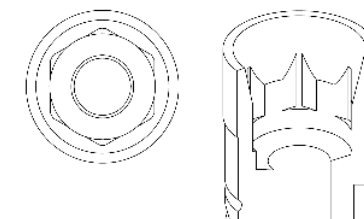

# COMPATIBLE with 0023

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			0,5 mm			mm			mm			mm		
R	31.322.023.01-2	45°	30°	31.322.023.02-2	25°	30°	-	-	-	-	-	-	-	-	-
NR	31.312.023.01-2			31.312.023.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.103.01-2	10	50.312.023.01-2	43.621.410.01-2	34.612.023.01-2	-	-	33.390.805.01-2	3	25°
			43.624.410.01-2				33.490.805.01-2	4	
52.412.103.01-2	12		43.630.410.01-2				33.690.805.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP				
41.316.059.01-2	-	43.618.201.01-2	18	40.316.008.01-2	43.601.108.01-2	22.612.023.01-2	30.412.001.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0023	LAB SCANBODY	DAS_C_E_0023
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0023	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0023
	DAS_I_12_0023		DAS_C_I_12_0023

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

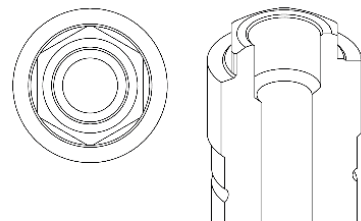

# COMPATIBLE with 0024

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			0,5 mm			mm			mm			mm		
R	31.323.024.01-2	45°	30°	31.323.024.02-2	30°	30°	-	-	-	-	-	-	-	-	-
NR	31.313.024.01-2			31.313.024.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®												
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	0,3 mm	CH=5mm	CH=7mm	CH=9mm	0,5 mm	CH=5mm	CH=7mm	CH=9mm	1 mm	CH=5mm	CH=7mm	CH=9mm
R	31.323.024.21-2	30°	25°	10°	31.323.024.22-2	30°	25°	10°	31.323.024.23-2	30°	25°	10°
NR	31.313.024.21-2				31.313.024.22-2				31.313.024.23-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.101.01-2	8	50.313.024.01-2	43.621.410.01-2	34.613.024.01-2	-	-	33.390.716.01-2	3	30°
52.410.101.01-2	10		43.624.410.01-2				33.490.716.01-2	4	
52.412.101.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP				
41.320.060.01-2	-	43.618.201.01-2	18	40.320.008.01-2	43.601.108.01-2	22.613.024.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0024	LAB SCANBODY	DAS_C_E_0024
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0024	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0024
	DAS_I_10_0024		DAS_C_I_10_0024
	DAS_I_12_0024		DAS_C_I_12_0024

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

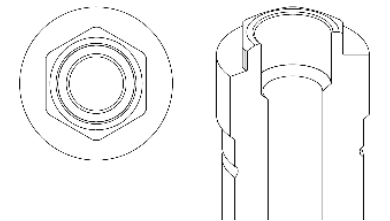



# COMPATIBLE with 0025

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			0,5 mm			mm			mm			mm		
R	31.323.025.01-2	45°	30°	31.323.025.02-2	30°	30°	-	-	-	-	-	-	-	-	-
NR	-			-			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	0,3 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.323.025.21-2	30°	25°	10°
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.408.112.01-2	8	50.313.025.02-2	43.620.411.01-2	34.613.025.01-2
52.410.111.01-2	10	50.313.025.01-2	43.621.410.01-2	
-	12		43.624.410.01-2	
			43.630.410.01-2	

DYNAMIC PRE-MILLED	
COBALT-CHROME	$\alpha_{dp}$
-	-

DYNAMIC MILLING TOOL		
DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
33.390.716.01-2	3	30°
33.490.716.01-2	4	
33.690.716.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.039.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS	
STRAIGHT SCREW	SCREWDRIVER UNIGRIP
40.314.008.01-2	43.601.108.01-2

ANALOG	LAB SCANBODY
22.613.025.01-2	30.413.005.01-2

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0025	LAB SCANBODY	DAS_C_E_0025
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_8_0025	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_8_0025
	DAS_I_10_0025		DAS_C_I_10_0025
	-		-

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

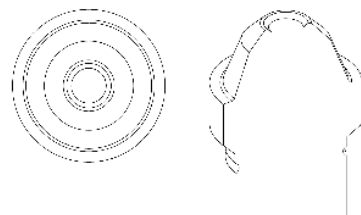

# COMPATIBLE with 0026

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			1,2 mm			mm			mm			mm		
R	31.322.026.01-2	45°	29°	31.322.026.02-2	25°	22°	-	-	-	-	-	-	-	-	-
NR	31.312.026.01-2			-			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	0,5 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.322.026.21-2	25°	20°	10°
NR	31.312.026.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG
52.410.108.01-2	10	50.312.026.01-2	43.621.410.01-2	34.612.026.01-2
			43.624.410.01-2	
52.412.108.01-2	12	43.630.410.01-2		

DYNAMIC PRE-MILLED	
COBALT-CHROME	$\alpha_{dp}$
-	-

DYNAMIC MILLING TOOL		
DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
33.390.805.01-2	3	25°
33.490.805.01-2	4	
33.690.805.01-2	6	

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.318.075.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS	
STRAIGHT SCREW	SCREWDRIVER UNIGRIP
40.318.008.01-2	43.601.108.01-2

ANALOG	LAB SCANBODY
22.612.026.01-2	30.412.001.01-2

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0026	LAB SCANBODY	DAS_C_E_0026
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0026	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0026
	DAS_I_12_0026		DAS_C_I_12_0026

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

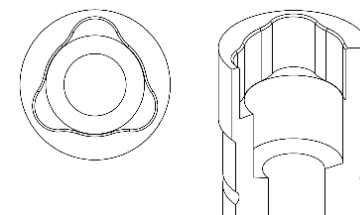

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			1,2 mm			mm			mm			mm		
R	31.323.027.01-2	39°	29°	31.323.027.02-2	25°	22°	-	-	-	-	-	-	-	-	-
NR	31.313.027.01-2			31.313.027.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	0,3 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.323.027.21-2	25°	20°	10°
NR	31.313.027.21-2			

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.109.01-2	10	50.313.027.01-2	43.621.410.01-2	34.613.027.01-2	-	-	33.390.958.01-2	3	30°
			43.624.410.01-2				33.490.958.01-2	4	
52.412.109.01-2	12		43.630.410.01-2				33.690.958.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP				
41.320.090.01-2	-	43.618.201.01-2	18	40.320.008.03-2	43.601.108.01-2	22.613.027.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0027	LAB SCANBODY	DAS_C_E_0027
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0027	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0027
	DAS_I_12_0027		DAS_C_I_12_0027

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

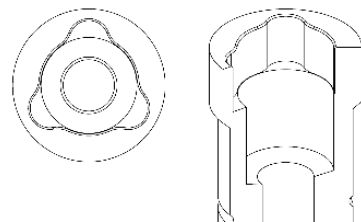

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			mm			mm			mm			mm		
R	31.324.028.01-2	38°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.028.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.109.01-2	10	50.314.028.01-2	43.621.410.01-2	34.614.028.01-2	-	-	33.390.958.01-2	3	30°
			43.624.410.01-2				33.490.958.01-2	4	
52.412.109.01-2	12		43.630.410.01-2				33.690.958.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP				
41.320.090.01-2	-	43.618.201.01-2	18	40.320.008.03-2	43.601.108.01-2	22.614.028.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0028	LAB SCANBODY	DAS_C_E_0028
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0028	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0028
	DAS_I_12_0028		DAS_C_I_12_0028

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

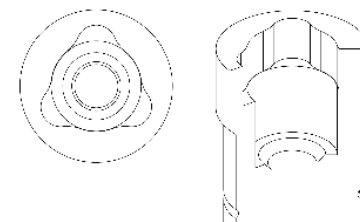

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,2 mm			2 mm			mm			4 mm			mm		
R	31.322.029.01-2	37°	23°	31.322.029.02-2	25°	15°	-	-	-	31.322.029.04-2	15°	25°	-	-	-
NR	31.312.029.01-2			31.312.029.02-2			-	-	31.312.029.04-2	-			-		

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.103.01-2	10	50.312.029.01-2	43.621.410.01-2	34.613.029.01-2	-	-	33.345.804.01-2	3	20°
			43.624.410.01-2				33.445.804.01-2	4	
52.412.103.01-2	12		43.630.410.01-2				33.645.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.316.094.01-2	41.316.132.01-2	43.618.201.01-2	18	40.316.003.02-2	43.601.103.02-2	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0029	LAB SCANBODY	DAS_C_E_0029
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0029	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0029
	DAS_I_12_0029		DAS_C_I_12_0029

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

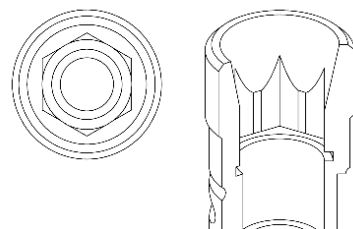

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,1 mm			2 mm			mm			4 mm			mm		
R	31.323.030.01-2	42°	25°	31.323.030.02-2	25°	15°	-	-	-	-	15°	30°	-	-	-
NR	31.313.030.01-2			31.313.030.02-2			-	-	31.313.030.04-2	-			-		

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	31.323.030.21-2	25°	20°	10°
NR	31.313.030.21-2			

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.101.01-2	8	50.313.030.01-2	43.621.410.01-2	34.613.030.01-2	-	-	33.345.808.01-2	3	30°
52.410.101.01-2	10		43.624.410.01-2				33.445.808.01-2	4	
52.412.101.01-2	12		43.630.410.01-2				33.645.808.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.320.079.01-2	41.320.125.01-2	43.618.201.01-2	18	40.320.003.04-2	43.601.103.02-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0030	LAB SCANBODY	DAS_C_E_0030
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_8_0030	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_8_0030
	DAS_I_10_0030		DAS_C_I_10_0030
	DAS_I_12_0030		DAS_C_I_12_0030

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

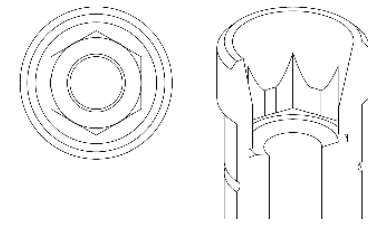

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.321.031.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.311.031.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.104.01-2	10	50.311.031.01-2	43.621.410.01-2	34.611.031.01-2	-	-	33.360.756.01-2	3	25°
			43.624.410.01-2				33.460.756.01-2	4	
52.412.104.01-2	12	43.630.410.01-2	33.660.756.01-2	6					

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER				
41.318.068.01-2	-	43.618.201.01-2	18	-	-	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0031	LAB SCANBODY	DAS_C_E_0031
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0031	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0031
	DAS_I_12_0031		DAS_C_I_12_0031

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

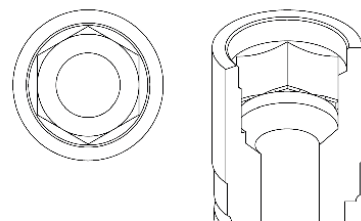

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,7 mm			mm			mm			mm			mm		
R	31.322.032.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.032.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.120.01-2	10	50.312.032.01-2	43.621.410.01-2	34.612.032.01-2	-	-	33.360.756.01-2	3	30°
			43.624.410.01-2				33.460.756.01-2	4	
52.412.120.01-2	12	43.630.410.01-2	33.660.756.01-2	6					

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER				
41.318.068.01-2	-	43.618.201.01-2	18	-	-	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0032	LAB SCANBODY	DAS_C_E_0032
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0032	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0032
	DAS_I_12_0032		DAS_C_I_12_0032

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

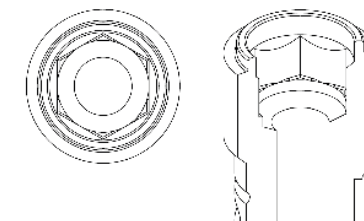



# COMPATIBLE with 0033

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,3 mm			2 mm			mm			mm			mm		
R	31.322.033.01-2	38°	18°	31.322.033.02-2	20°	14°	-	-	-	-	-	-	-	-	-
NR	31.312.033.01-2			31.312.033.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	1,3 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.322.033.21-2	25°	20°	10°
NR	31.312.033.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.106.01-2	8	50.312.033.01-2	43.621.410.01-2	34.612.033.01-2	32.212.033.02-2	25°	33.315.804.01-2	3	25°
52.410.106.01-2	10		43.624.410.01-2				33.415.804.01-2	4	
52.412.106.01-2	12		43.630.410.01-2				33.615.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.316.078.01-2	-	43.618.201.01-2	18	40.316.007.01-2	43.601.107.01-2	22.612.033.01-2	30.412.001.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0033	LAB SCANBODY	DAS_C_E_0033
	DAS_I_8_0033		DAS_C_I_8_0033
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0033	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0033
	DAS_I_12_0033		DAS_C_I_12_0033

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

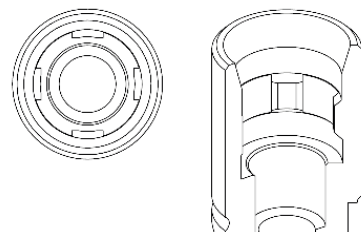

# COMPATIBLE with 0035

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,1 mm			2 mm			mm			mm			mm		
R	31.323.035.01-2	39°	18°	31.323.035.02-2	20°	14°	-	-	-	-	-	-	-	-	-
NR	31.313.035.01-2			31.313.035.02-2			-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	1,1 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.323.035.21-2	25°	20°	10°
NR	31.313.035.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.107.01-2	10	50.313.035.01-2	43.621.410.01-2	34.613.035.01-2	32.213.035.02-2	25°	33.315.804.01-2	3	25°
			43.624.410.01-2				33.415.804.01-2	4	
52.412.107.01-2	12		43.630.410.01-2				33.615.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.316.078.01-2	-	43.618.201.01-2	18	40.316.007.01-2	43.601.107.01-2	22.613.035.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0035	LAB SCANBODY	DAS_C_E_0035
	DAS_I_10_0035		DAS_C_I_10_0035
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_12_0035	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_12_0035

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

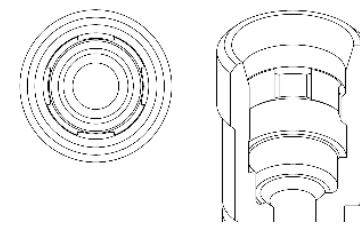

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.323.037.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.037.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.110.01-2	10	50.313.037.01-2	43.621.410.01-2	34.613.037.01-2	32.213.037.02-2	30°	33.315.708.01-2	3	30°
			43.624.410.01-2				33.415.708.01-2	4	
52.412.110.01-2	12		43.630.410.01-2				33.615.708.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.320.067.01-2	-	43.618.201.01-2	18	40.320.007.01-2	43.601.107.01-2	22.613.037.01-2	30.413.004.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0037	LAB SCANBODY	DAS_C_E_0037
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0037	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0037
	DAS_I_12_0037		DAS_C_I_12_0037

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

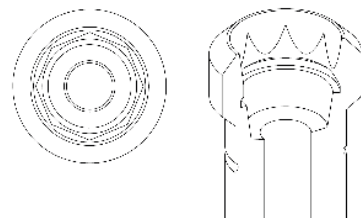

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,7 mm			mm			mm			mm			mm		
R	31.322.038.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.038.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	30°	25°	10°
NR	31.312.038.21-2			

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.103.01-2	10	50.312.038.01-2	43.621.410.01-2	34.612.038.01-2	-	-	33.345.804.01-2	3	25°
			43.624.410.01-2				33.445.804.01-2	4	
52.412.103.01-2	12		43.630.410.01-2				33.645.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25				
41.316.081.01-2	-	43.618.201.01-2	18	40.316.004.02-2	43.601.104.01-2	22.613.037.01-2	30.413.004.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0038	LAB SCANBODY	DAS_C_E_0038
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0038	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0038
	DAS_I_12_0038		DAS_C_I_12_0038

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

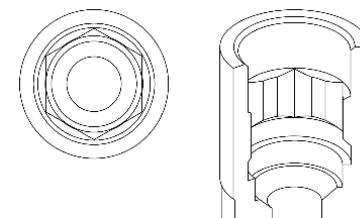

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,7 mm			mm			mm			mm			mm		
R	31.323.039.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.039.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	0,7 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.323.039.21-2	30°	25°	10°
NR	31.313.039.21-2			

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.114.01-2	10	50.313.039.01-2	43.621.410.01-2	34.613.039.01-2	-	-	33.345.856.01-2	3	25°
			43.624.410.01-2				33.445.856.01-2	4	
52.412.114.01-2	12		43.630.410.01-2				33.645.856.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25				
41.316.081.01-2	-	43.618.201.01-2	18	40.316.004.02-2	43.601.104.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0039	LAB SCANBODY	DAS_C_E_0039
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0039	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0039
	DAS_I_12_0039		DAS_C_I_12_0039

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

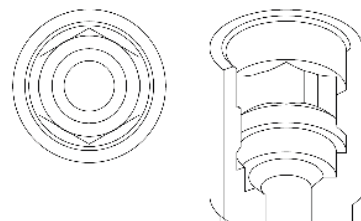

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			1,5 mm			3 mm			mm			5 mm		
R	31.322.040.01-2	45°	30°	31.322.040.02-2	25°	25°	31.322.040.03-2	20°	30°	-	-	-	31.322.040.05-2	10°	23°
NR	31.312.040.01-2			31.312.040.02-2			31.312.040.03-2			31.312.040.05-2					
NR (Friction-Fit)	31.312.042.01-2			-			-			-					

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	0,6 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.322.040.21-2	25°	20°	10°
NR	31.312.040.21-2			

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.101.01-2	8	50.312.040.01-2	43.621.410.01-2	34.612.040.01-2	32.212.040.02-2	25°	33.370.716.01-2	3	25°
52.410.101.01-2	10		43.624.410.01-2				33.470.716.01-2	4	
52.412.101.01-2	12		43.630.410.01-2				33.670.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.317.071.01-2	41.317.106.01-2	43.618.201.01-2	18	40.317.004.01-2	43.601.104.01-2	-	-	22.612.040.01-2	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0040	LAB SCANBODY	DAS_C_E_0040
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_8_0040	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_8_0040
	DAS_I_10_0040		DAS_C_I_10_0040
	DAS_I_12_0040		DAS_C_I_12_0040

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

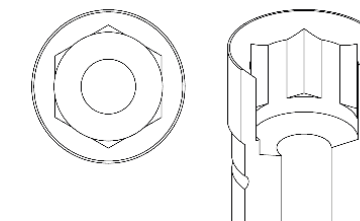

# COMPATIBLE with 0040b

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			1,5 mm			3 mm			mm			5 mm		
R	31.322.040.01-2	45°	30°	31.322.040.02-2	25°	25°	31.322.040.03-2	20°	30°	-	-	-	31.322.040.05-2	10°	25°
NR	31.312.040.01-2			31.312.040.02-2			31.312.040.03-2			31.312.040.05-2					

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	0,6 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.322.040.21-2	25°	20°	10°
NR	31.312.040.21-2			

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	32.212.040.02-2	25°	33.370.716.01-2	3	25°
-	-	-	-	-			33.470.716.01-2	4	
-	-	-	-	-			33.670.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.318.071.01-2	-	43.618.201.01-2	18	-	-	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0040	LAB SCANBODY	DAS_C_E_0040
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-
	-		-

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

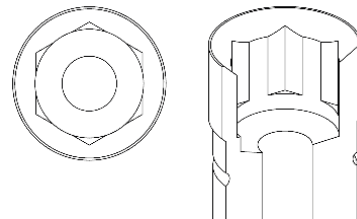

# COMPATIBLE with 0041

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,4 mm			1,5 mm			mm			mm			mm		
R	31.323.041.01-2	45°	30°	31.323.041.02-2	30°	25°	-	-	-	-	-	-	-	-	-
NR	31.313.041.01-2			31.313.041.02-2			-			-					
NR (Friction-Fit)	31.313.043.01-2			-			-			-					

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	0,4 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.323.041.21-2	30°	20°	10°
NR	31.313.041.21-2			

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.102.01-2	10	50.313.041.01-2	43.621.410.01-2	34.613.041.01-2	32.013.041.02-2	30°	33.370.716.01-2	3	30°
			43.624.410.01-2				33.470.716.01-2	4	
52.412.102.01-2	12		43.630.410.01-2				33.670.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.317.071.01-2	-	43.618.201.01-2	18	40.317.004.01-2	43.601.104.01-2	22.613.041.01-2	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0041	LAB SCANBODY	DAS_C_E_0041
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0041	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0041
	DAS_I_12_0041		DAS_C_I_12_0041

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

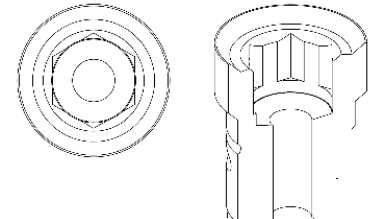



# COMPATIBLE with 0041b

## STANDARD DYNAMIC TIBASE®

	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,4 mm			1,5 mm			mm			mm			mm		
R	31.323.041.01-2	45°	30°	31.323.041.02-2	30°	25°	-	-	-	-	-	-	-	-	-
NR	31.313.041.01-2			31.313.041.02-2			-	-	-	-	-	-	-	-	-

## DYNAMIC 3TIBASE®

	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	0,4 mm	CH=5mm	CH=7mm	CH=9mm
R	31.323.041.21-2	30°	20°	10°
NR	31.313.041.21-2			

## DYNAMIC μSCANBODY (LAB/CLIN)

## DIGITAL ANALOG

## DYNAMIC PRE-MILLED

## DYNAMIC MILLING TOOL

SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	32.013.041.02-2	30°	33.370.716.01-2	3	30°
-	-	-	-	-			33.470.716.01-2	4	
-	-	-	-	-			33.670.716.01-2	6	

## DYNAMIC μSCANBODY (LAB/CLIN)

## DIGITAL ANALOG

## DYNAMIC PRE-MILLED

## DYNAMIC MILLING TOOL

SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.105.01-2	10	50.312.044.01-2	43.621.410.01-2	34.612.044.01-2	-	-	33.390.716.01-2	3	25°
			43.624.410.01-2			33.490.716.01-2	4		
52.412.105.01-2	12	43.630.410.01-2		33.690.716.01-2	6				

## DYNAMIC SCREWS

## STRAIGHT SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27	ANALOG	LAB SCANBODY
41.318.071.01-2	-	43.618.201.01-2	18	-	-	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

## DYNAMIC SCREWS

## STRAIGHT SCREWS

DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.318.065.01-2	-	43.618.201.01-2	18	40.318.003.01-2	43.601.103.02-2	-	30.412.001.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0041	LAB SCANBODY	DAS_C_E_0041
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

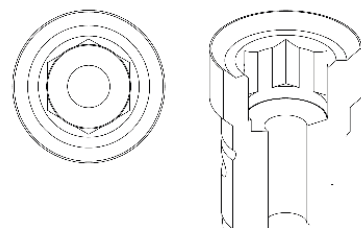

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0044	LAB SCANBODY	DAS_C_E_0044
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0044	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0044
	DAS_I_12_0044		DAS_C_I_12_0044

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

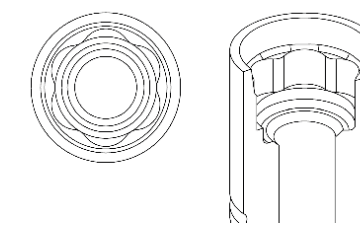

# COMPATIBLE with 0044

## STANDARD DYNAMIC TIBASE®

	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1 mm			mm			mm			mm			mm		
R	31.322.044.01-2	42°	23°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.044.01-2			-			-			-			-		

## DYNAMIC 3TIBASE®

	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	1 mm	CH=5mm	CH=7mm	CH=9mm
R	31.322.044.21-2	25°	20°	10°
NR	31.312.044.21-2			

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1 mm			mm			mm			mm			mm		
R	31.323.045.01-2	43°	22°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.045.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	1 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.323.045.21-2	30°	20°	10°
NR	31.313.045.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.118.01-2	10	50.313.045.01-2	43.621.410.01-2	34.613.045.01-2	-	-	33.390.716.01-2	3	30°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.118.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.318.065.01-2	-	43.618.201.01-2	18	40.318.003.01-2	43.601.103.02-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0045	LAB SCANBODY	DAS_C_E_0045
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0045	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0045
	DAS_I_12_0045		DAS_C_I_12_0045

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

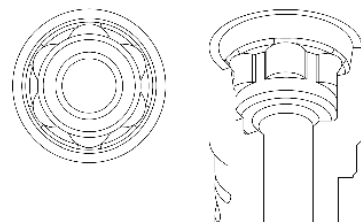

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1 mm			mm			mm			mm			mm		
R	31.324.046.01-2	42°	21°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.046.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	1 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.324.046.21-2	30°	20°	10°
NR	-			

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.125.01-2	10	50.314.046.01-2	43.621.410.01-2	34.614.046.01-2	-	-	33.390.716.01-2	3	30°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.125.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.318.065.01-2	-	43.618.201.01-2	18	40.318.003.01-2	43.601.103.02-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0046	LAB SCANBODY	DAS_C_E_0046
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0046	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0046
	DAS_I_12_0046		DAS_C_I_12_0046

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

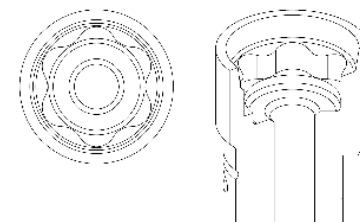

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.322.047.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.047.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.123.01-2	10	50.312.047.01-2	43.621.410.01-2	34.612.047.01-2	-	-	33.390.716.01-2	3	25°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.123.01-2	12	43.630.410.01-2	33.690.716.01-2	6					

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.320.074.01-2	-	43.618.201.01-2	18	40.320.007.02-2	43.601.107.01-2	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0047	LAB SCANBODY	DAS_C_E_0047
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0047	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0047
	DAS_I_12_0047		DAS_C_I_12_0047

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

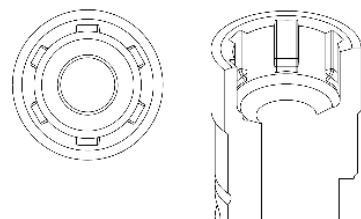

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.323.048.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.048.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.123.01-2	10	50.312.047.01-2	43.621.410.01-2	34.612.047.01-2	-	-	33.390.716.01-2	3	30°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.123.01-2	12	43.630.410.01-2	33.690.716.01-2	6					

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.320.074.01-2	-	43.618.201.01-2	18	40.320.007.02-2	43.601.107.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0048	LAB SCANBODY	DAS_C_E_0048
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0048	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0048
	DAS_I_12_0048		DAS_C_I_12_0048

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

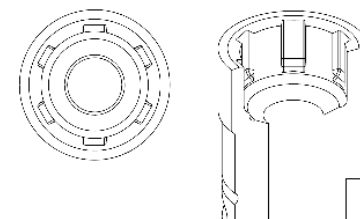

# COMPATIBLE with 0049

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.321.049.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.311.049.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.116.01-2	10	50.311.049.01-2	43.621.410.01-2	34.611.049.01-2	-	-	33.325.472.01-2	3	25°
			43.624.410.01-2				33.425.472.01-2	4	
52.412.116.01-2	12		43.630.410.01-2				33.625.472.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25				
41.314.064.01-2	-	43.618.201.01-2	18	40.314.004.01-2	43.601.104.01-2	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0049	LAB SCANBODY	DAS_C_E_0049
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0049	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0049
	DAS_I_12_0049		DAS_C_I_12_0049

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

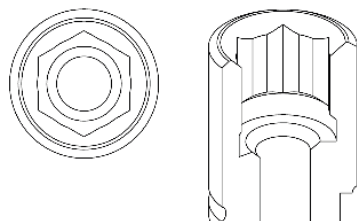

# COMPATIBLE with 0050

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.323.051.01-2	45°	27°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.051.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.117.01-2	10	50.312.050.01-2	43.621.410.01-2	34.612.050.01-2	-	-	33.335.676.01-2	3	25°
			43.624.410.01-2				33.435.676.01-2	4	
52.412.117.01-2	12		43.630.410.01-2				33.635.676.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25				
41.318.064.01-2	-	43.618.201.01-2	18	40.318.004.03-2	43.601.104.01-2	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0050	LAB SCANBODY	DAS_C_E_0050
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0050	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0050
	DAS_I_12_0050		DAS_C_I_12_0050

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

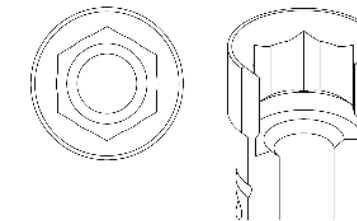



# COMPATIBLE with 0051

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.323.051.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.051.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.118.01-2	10	50.313.051.01-2	43.621.410.01-2	34.613.051.01-2	-	-	33.335.676.01-2	3	25°
			43.624.410.01-2				33.435.676.01-2	4	
52.412.118.01-2	12		43.630.410.01-2				33.635.676.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25				
41.318.064.01-2	-	43.618.201.01-2	18	40.318.004.03-2	43.601.104.01-2	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0051	LAB SCANBODY	DAS_C_E_0051
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0051	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0051
	DAS_I_12_0051		DAS_C_I_12_0051

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

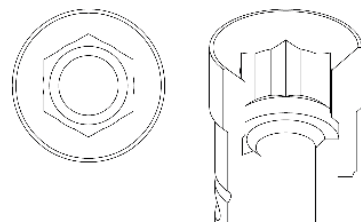

# COMPATIBLE with 0052

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			mm			mm			mm			mm		
R	31.324.052.01-2	45°	27°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.052.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.102.01-2	10	50.314.052.01-2	43.621.410.01-2	34.614.052.01-2	-	-	33.335.676.01-2	3	30°
			43.624.410.01-2				33.435.676.01-2	4	
52.412.102.01-2	12		43.630.410.01-2				33.635.676.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25				
41.318.064.01-2	-	43.618.201.01-2	18	40.318.004.03-2	43.601.104.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0052	LAB SCANBODY	DAS_C_E_0052
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0052	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0052
	DAS_I_12_0052		DAS_C_I_12_0052

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

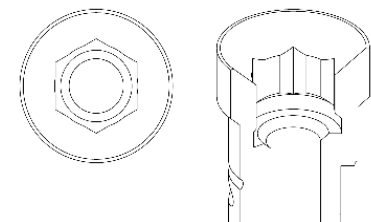

# COMPATIBLE with 0054

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.323.054.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.054.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.119.01-2	10	50.314.054.01-2	43.621.410.01-2	34.614.054.01-2	-	-	33.345.856.01-2	3	30°
			43.624.410.01-2				33.445.856.01-2	4	
52.412.119.01-2	12		43.630.410.01-2				33.645.856.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Star 1.50				
41.318.067.01-2	-	43.618.201.01-2	18	40.318.012.01-2	-	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0054	LAB SCANBODY	DAS_C_I_0054
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0054	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0054
	DAS_I_12_0054		DAS_C_I_12_0054

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

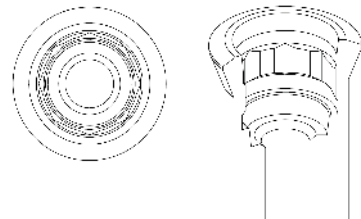

# COMPATIBLE with 0057

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.324.057.01-2	45°	27°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.057.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.101.01-2	8	50.314.057.01-2	43.621.410.01-2	34.614.057.01-2	-	-	33.390.805.01-2	3	30°
52.410.101.01-2	10		43.624.410.01-2				33.490.805.01-2	4	
52.412.101.01-2	12		43.630.410.01-2				33.690.805.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.316.084.01-2	-	43.618.201.01-2	18	40.316.003.01-2	43.601.103.02-2	22.614.057.01-2	30.414.003.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0057	LAB SCANBODY	DAS_C_E_0057
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_8_0057	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_8_0057
	DAS_I_10_0057		DAS_C_I_10_0057
	DAS_I_12_0057		DAS_C_I_12_0057

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

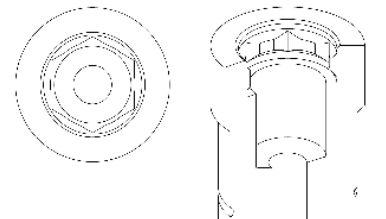

# COMPATIBLE with 0058

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.324.058.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.058.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.118.01-2	10	50.314.058.01-2	43.621.410.01-2	34.614.058.01-2	-	-	33.390.716.01-2	3	30°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.118.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.320.047.01-2	-	43.618.201.01-2	18	40.320.003.01-2	43.601.103.02-2	22.614.058.01-2	30.414.003.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0058	LAB SCANBODY	DAS_C_E_0058
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0058	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0058
	DAS_I_12_0058		DAS_C_I_12_0058

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

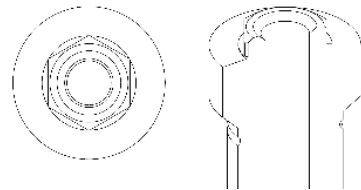

# COMPATIBLE with 0059

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,7 mm			mm			mm			mm			mm		
R	31.324.059.01-2	45°	27°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.059.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	-	-
							-	-	
-	-						-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.318.065.01-2	-	43.618.201.01-2	18	40.318.003.01-2	43.601.103.02-2	22.614.059.01-2	30.414.003.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0059	LAB SCANBODY	DAS_C_E_0059
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

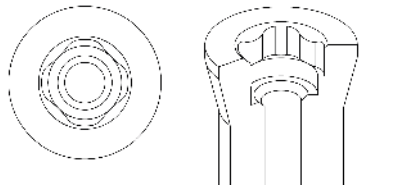

# COMPATIBLE with 0060

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.324.060.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.060.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.122.01-2	10	50.314.060.01-2	43.621.410.01-2	34.614.060.01-2	-	-	33.390.716.01-2	3	30°
			43.624.410.01-2				33.490.716.01-2	4	
52.412.122.01-2	12		43.630.410.01-2				33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20				
41.320.060.01-2	-	43.618.201.01-2	18	40.320.003.02-2	43.601.103.02-2	22.614.060.01-2	30.415.007.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0060	LAB SCANBODY	DAS_C_E_0060
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0060	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0060
	DAS_I_12_0060		DAS_C_I_12_0060

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

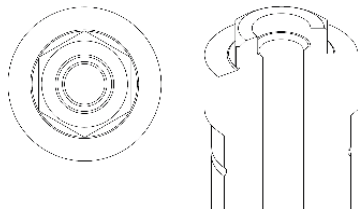

# COMPATIBLE with 0061

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.324.061.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.061.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.125.01-2	10	50.314.061.01-2	43.621.410.01-2	34.614.061.01-2	-	-	33.390.958.01-2	3	30°
			43.624.410.01-2				33.490.958.01-2	4	
52.412.125.01-2	12		43.630.410.01-2				33.690.958.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP				
41.325.067.01-2	-	43.618.201.01-2	18	40.325.008.01-2	43.601.108.01-2	22.614.061.01-2	30.415.007.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0061	LAB SCANBODY	DAS_C_E_0061
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0061	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0061
	DAS_I_12_0061		DAS_C_I_12_0061

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

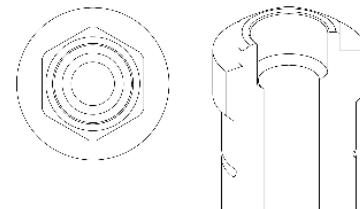

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.322.063.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.063.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	33.360.756.01-2	3	25°
-	-	-	-	-	-	-	-	33.460.756.01-2	4	
-	-	-	-	-	-	-	-	33.660.756.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER				
41.318.051.01-2	-	43.618.201.01-2	18	-	-	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0063	LAB SCANBODY	DAS_C_E_0063
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

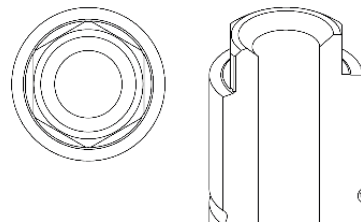

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.323.064.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.064.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.101.01-2	8	50.313.064.01-2	43.621.410.01-2			-	-	33.360.756.01-2	3	30°
52.410.101.01-2	10		43.624.410.01-2					33.460.756.01-2	4	
52.412.101.01-2	12		43.630.410.01-2					33.660.756.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER				
41.320.048.01-2	-	43.618.201.01-2	18	-	-	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0064	LAB SCANBODY	DAS_C_E_0064
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

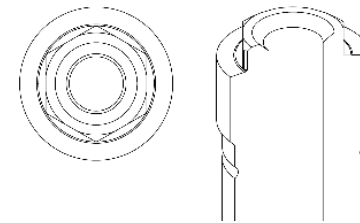



STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,9 mm			mm			mm			mm			mm		
R	31.323.065.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.065.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.121.01-2	10	50.313.065.01-2	43.621.410.01-2	34.613.065.01-2	-	-	33.360.756.01-2	3	30°
			43.624.410.01-2				33.460.756.01-2	4	
52.412.121.01-2	12		43.630.410.01-2				33.660.756.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER			
41.320.068.01-2	-	43.618.201.01-2	18	-	-	-	-	30.413.002.01-2
		43.624.201.01-2	24					
		43.632.201.01-2	32					

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0065	LAB SCANBODY	DAS_C_E_0065
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0065	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0065
	DAS_I_12_0065		DAS_C_I_12_0065

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

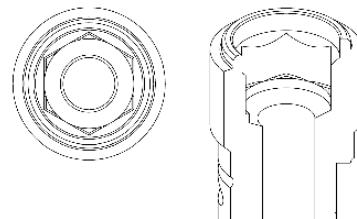

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.323.066.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	-	-
							-	-	
-	-						-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER			
41.314.039.01-2	-	43.618.201.01-2	18	-	-	-	-	30.412.001.01-2
		43.624.201.01-2	24					
		43.632.201.01-2	32					

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0066	LAB SCANBODY	DAS_C_E_0066
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

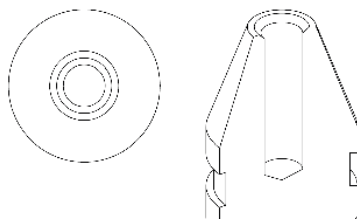

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.323.074.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.074.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.110.01-2	10	50.313.074.01-2	43.621.410.01-2	34.613.074.01-2	-	-	33.330.708.01-2	3	30°
			43.624.410.01-2				33.430.708.01-2	4	
52.412.110.01-2	12		43.630.410.01-2				33.630.708.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Sq. 1.30				
41.320.044.01-2	-	43.618.201.01-2	18	40.320.007.04-2	43.601.102.01-2	22.613.074.01-2	30.415.007.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0074	LAB SCANBODY	DAS_C_E_0074
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0074	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0074
	DAS_I_12_0074		DAS_C_I_12_0074

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

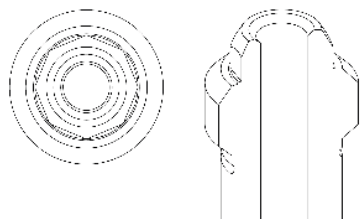

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1 mm			2 mm			mm			mm			mm		
R	31.322.075.01-2	42°	24°	31.322.075.02-2	25°	15°	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.105.01-2	10	50.312.075.01-2	43.621.410.01-2	34.612.075.01-2	-	-	33.330.734.01-2	3	25°
			43.624.410.01-2				33.430.734.01-2	4	
52.412.105.01-2	12		43.630.410.01-2				33.630.734.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.00				
41.318.077.01-2	-	43.618.201.01-2	18	40.318.013.01-2	-	22.612.075.01-2	30.412.001.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0075	LAB SCANBODY	DAS_C_E_0075
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0075	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0075
	DAS_I_12_0075		DAS_C_I_12_0075

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

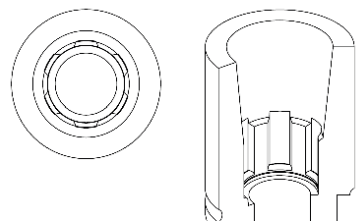

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,4 mm			mm			mm			mm			mm		
R	31.324.080.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.080.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.124.01-2	10	50.314.080.01-2	43.621.410.01-2	34.614.080.01-2	-	-	33.370.716.01-2	3	30°
			43.624.410.01-2				33.470.716.01-2	4	
52.412.124.01-2	12		43.630.410.01-2				33.670.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.317.071.01-2	-	43.618.201.01-2	18	40.317.004.01-2	43.601.104.01-2	22.614.080.01-2	30.414.003.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0080	LAB SCANBODY	DAS_C_E_0080
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0080	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0080
	DAS_I_12_0080		DAS_C_I_12_0080

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

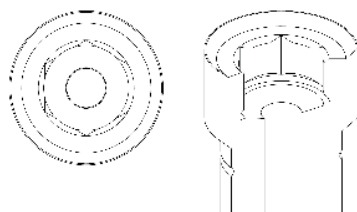

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,4 mm			mm			mm			mm			mm		
R	31.325.081.01-2	41°	18°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.315.081.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.126.01-2	10	50.315.081.01-2	43.621.410.01-2	34.615.081.01-2	-	-	33.335.676.01-2	3	30°
			43.624.410.01-2				33.435.676.01-2	4	
52.412.126.01-2	12		43.630.410.01-2				33.635.676.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25				
41.318.064.01-2	-	43.618.201.01-2	18	40.318.004.03-2	43.601.104.01-2	22.614.080.01-2	30.414.003.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0081	LAB SCANBODY	DAS_C_E_0081
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0081	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0081
	DAS_I_12_0081		DAS_C_I_12_0081

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

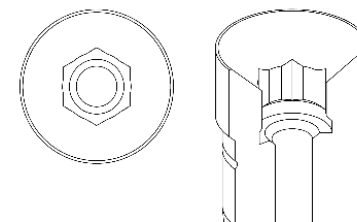

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,2 mm			mm			mm			mm			mm		
R	31.322.082.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.082.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.105.01-2	10	50.312.082.01-2	43.621.410.01-2	34.612.082.01-2	-	-	33.345.804.01-2	3	25°
			43.624.410.01-2				33.445.804.01-2	4	
52.412.105.01-2	12		43.630.410.01-2				33.645.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Star 1.50				
41.316.074.01-2	-	43.618.201.01-2	18	40.316.012.01-2	-	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0082	LAB SCANBODY	DAS_C_E_0082
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0082	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0082
	DAS_I_12_0082		DAS_C_I_12_0082

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

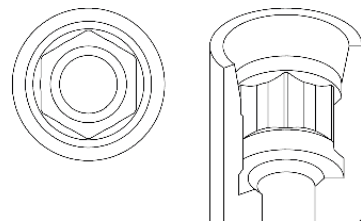

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,2 mm			mm			mm			mm			mm		
R	31.323.083.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.083.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.103.01-2	10	50.313.083.01-2	43.621.410.01-2	34.613.083.01-2	-	-	33.345.856.01-2	3	30°
			43.624.410.01-2				33.445.856.01-2	4	
52.412.103.01-2	12		43.630.410.01-2				33.645.856.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Star 1.50				
41.318.076.01-2	-	43.618.201.01-2	18	40.318.012.02-2	-	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0083	LAB SCANBODY	DAS_C_E_0083
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0083	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0083
	DAS_I_12_0083		DAS_C_I_12_0083

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

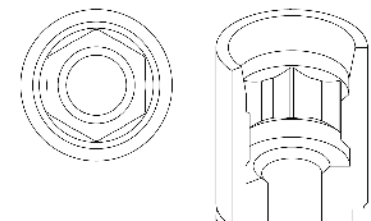

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			mm			mm			mm			mm		
R	31.324.085.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.085.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.117.01-2	10	50.314.085.01-2	43.621.410.01-2	34.614.085.01-2	-	-	33.345.856.01-2	3	25°
			43.624.410.01-2				33.445.856.01-2	4	
52.412.117.01-2	12	43.630.410.01-2	33.645.856.01-2	6					

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25				
41.316.081.01-2	-	43.618.201.01-2	18	40.316.004.02-2	43.601.104.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0085	LAB SCANBODY	DAS_C_E_0085
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0085	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0085
	DAS_I_12_0085		DAS_C_I_12_0085

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

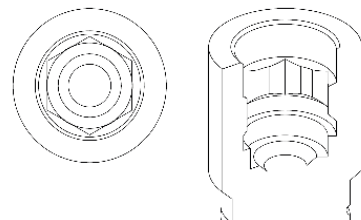

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1 mm			mm			mm			mm			mm		
R	31.321.090.01-2	45°	24°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.311.090.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.128.01-2	10	50.311.090.01-2	43.621.415.01-2	34.611.090.01-2	-	-	33.325.472.01-2*	3	25°
							33.425.472.01-2*	4	
52.412.128.01-2	12	33.625.472.01-2*	6						

\*Only for R

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.314.074.01-2	-	43.618.201.01-2	18	40.314.005.01-2	43.601.105.01-2	-	-	-	22.611.090.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0090	LAB SCANBODY	DAS_C_E_0090
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0090	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0090
	DAS_I_12_0090		DAS_C_I_12_0090

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

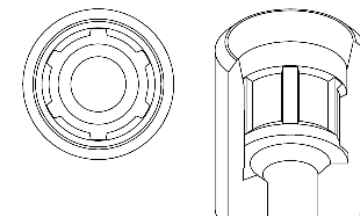



# COMPATIBLE with 0091

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,2 mm			mm			mm			mm			mm		
R	31.324.091.01-2	38°	18°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.091.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.102.01-2	10	50.314.091.01-2	43.621.410.01-2	34.614.091.01-2	-	-	33.390.958.01-2	3	30°
			43.624.410.01-2				33.490.958.01-2	4	
52.412.102.01-2	12	43.630.410.01-2	33.690.958.01-2	6					

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.320.082.01-2	-	43.618.201.01-2	18	40.320.005.01-2	43.601.105.01-2	22.614.091.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0091	LAB SCANBODY	DAS_C_E_0091
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0091	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0091
	DAS_I_12_0091		DAS_C_I_12_0091

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

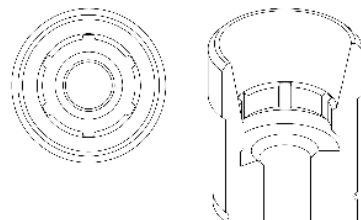

# COMPATIBLE with 0092

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1 mm			mm			mm			mm			mm		
R	31.325.092.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.315.092.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.129.01-2	10	50.315.092.01-2	43.621.410.01-2	34.615.092.01-2	-	-	33.390.958.01-2	3	30°
			43.624.410.01-2				33.490.958.01-2	4	
52.412.129.01-2	12	43.630.410.01-2	33.690.958.01-2	6					

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.320.082.01-2	-	43.618.201.01-2	18	40.320.005.01-2	43.601.105.01-2	22.615.092.01-2	30.415.007.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0092	LAB SCANBODY	DAS_C_E_0092
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0092	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0092
	DAS_I_12_0092		DAS_C_I_12_0092

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

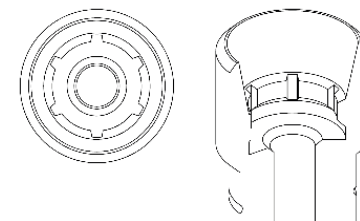

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.324.096.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.096.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.110.01-2	10	50.314.096.01-2	43.621.410.01-2	34.614.096.01-2	-	-	33.315.708.01-2	3	30°
			43.624.410.01-2				33.415.708.01-2	4	
52.412.110.01-2	12		43.630.410.01-2				33.615.708.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.320.067.01-2	-	43.618.201.01-2	18	40.320.007.01-2	43.601.107.01-2	22.614.096.01-2	30.414.008.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0096	LAB SCANBODY	DAS_C_E_0096
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0096	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0096
	DAS_I_12_0096		DAS_C_I_12_0096

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

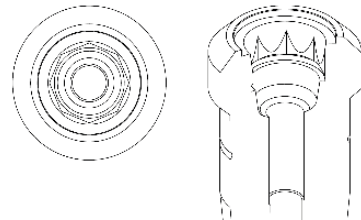

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.323.101.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	-	-
							-	-	
-	-						-	-	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.314.043.01-2	-	43.618.201.01-2	18	40.314.007.01-2	43.601.107.01-2	22.614.096.01-2	30.413.005.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0101	LAB SCANBODY	DAS_C_E_0101
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

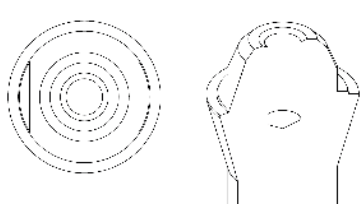

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,8 mm			mm			mm			mm			mm		
R	31.322.102.01-2	38°	18°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.102.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
	1,8 mm	CH=5mm	CH= 7mm	CH= 9mm
R	31.322.102.21-2	25°	15°	10°
NR	31.312.102.21-2			

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	
-	-	-	-	-	-
-	-	-	-	-	-

DYNAMIC PRE-MILLED	
COBALT-CHROME	$\alpha_{dp}$
-	-

DYNAMIC MILLING TOOL		
DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-
-	-	-

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.317.065.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS	
STRAIGHT SCREW	SCREWDRIVER Hex. 1.27
40.317.005.02-2	43.601.105.01-2

ANALOG	LAB SCANBODY
-	30.412.001.01-2

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0102	LAB SCANBODY	DAS_C_E_0102
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

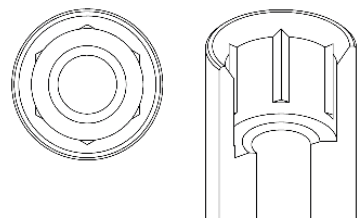

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,2 mm			mm			mm			mm			mm		
R	31.322.109.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.109.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	
52.410.128.01-2	10	50.312.109.01-2	43.621.415.01-2	34.612.109.01-2	-
-	-				-
52.412.128.01-2	12				-

DYNAMIC PRE-MILLED	
COBALT-CHROME	$\alpha_{dp}$
-	-

DYNAMIC MILLING TOOL		
DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
33.360.754.01-2*	3	25°
33.460.754.01-2*	4	
33.660.754.01-2*	6	

\*Only for R

DYNAMIC SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)
41.314.070.01-2	-	43.618.201.01-2	18
		43.624.201.01-2	24
		43.632.201.01-2	32

STRAIGHT SCREWS	
STRAIGHT SCREW	SCREWDRIVER Hex. 1.27
40.314.005.02-2	43.601.105.01-2

ANALOG	LAB SCANBODY
22.612.109.01-2	30.412.001.01-2

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0109	LAB SCANBODY	DAS_C_E_0109
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0109	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0109
	DAS_I_12_0109		DAS_C_I_12_0109

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

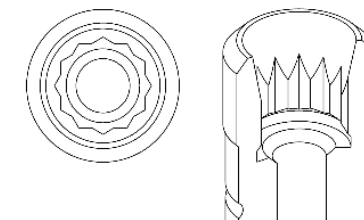

# COMPATIBLE with 0110

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,4 mm			mm			mm			mm			mm		
R	31.320.110.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.110.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-	-	-


DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.318.083.01-2	-	43.618.201.01-2	18	40.318.007.01-2	43.601.107.01-2	-	-	-	30.410.006.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES			
STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0110	LAB SCANBODY	DAS_C_E_0110
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-

**LIBRARY OPTIONS**  
**GH** = Gingival Height  
**CH** = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

**R** = Rotational / Non-Engaging  
**NR** = Non Rotational / Engaging

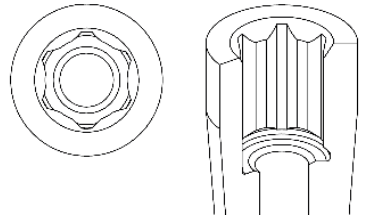

# COMPATIBLE with 0111

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,4 mm			mm			mm			mm			mm		
R	31.323.111.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.111.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH= 7mm	CH= 9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-	-	-


DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.318.083.01-2	-	43.618.201.01-2	18	40.318.007.01-2	43.601.107.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES			
STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0111	LAB SCANBODY	DAS_C_E_0111
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-

**LIBRARY OPTIONS**  
**GH** = Gingival Height  
**CH** = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

**R** = Rotational / Non-Engaging  
**NR** = Non Rotational / Engaging

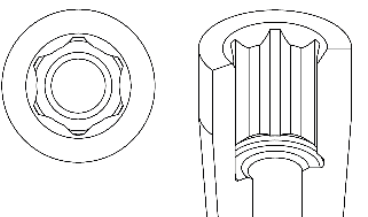

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1 mm			mm			mm			mm			mm		
R	31.323.121.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.121.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$
52.410.108.01-2	10	50.312.120.01-2	43.621.410.01-2	34.612.120.01-2	-	-
			43.624.410.01-2			
52.412.108.01-2	12		43.630.410.01-2			

DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
33.360.754.01-2	3	20°
33.460.754.01-2	4	
33.660.754.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.080.01-2	-	43.618.201.01-2	18	40.316.005.07-2	43.601.105.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0120	LAB SCANBODY	DAS_C_E_0120
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0120	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0120
	DAS_I_12_0120		DAS_C_I_12_0120

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

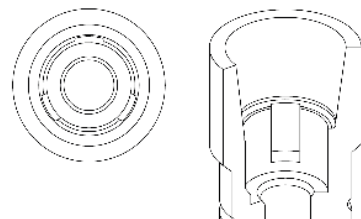

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1 mm			mm			mm			mm			mm		
R	31.323.121.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.121.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$
52.410.109.01-2	10	50.313.121.01-2	43.621.410.01-2	34.613.121.01-2	-	-
			43.624.410.01-2			
52.412.109.01-2	12		43.630.410.01-2			

DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
33.360.754.01-2	3	20°
33.460.754.01-2	4	
33.660.754.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.080.01-2	-	43.618.201.01-2	18	40.316.005.07-2	43.601.105.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0121	LAB SCANBODY	DAS_C_E_0121
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0121	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0121
	DAS_I_12_0121		DAS_C_I_12_0121

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

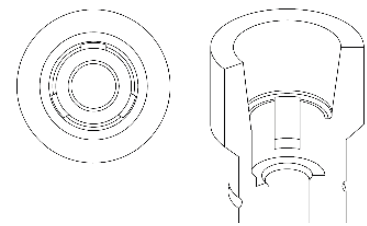



# COMPATIBLE with 0124

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,4 mm			mm			mm			mm			mm		
R	31.324.124.01-2	42°	19°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.124.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.125.01-2	10	50.314.124.01-2	43.621.410.01-2	34.614.124.01-2	-	-	33.335.758.01-2	3	30°
			43.624.410.01-2				33.435.758.01-2	4	
52.412.125.01-2	12		43.630.410.01-2				33.635.758.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP				
41.320.075.01-2	-	43.618.201.01-2	18	40.320.008.02-2	43.601.108.01-2	22.614.124.01-2	30.414.003.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0124	LAB SCANBODY	DAS_C_E_0124
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0124	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0124
	DAS_I_12_0124		DAS_C_I_12_0124

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

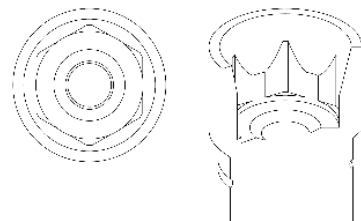

# COMPATIBLE with 0125

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,1 mm			mm			mm			mm			mm		
R	31.323.125.01-2	42°	20°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.125.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.117.01-2	10	50.313.125.01-2	43.621.410.01-2	34.613.125.01-2	-	-	33.315.804.01-2	3	25°
			43.624.410.01-2				33.415.804.01-2	4	
52.412.117.01-2	12		43.630.410.01-2				33.615.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.316.078.01-2	-	43.618.201.01-2	18	40.316.007.01-2	43.601.107.01-2	22.614.124.01-2	30.413.002.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0125	LAB SCANBODY	DAS_C_E_0125
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0125	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0125
	DAS_I_12_0125		DAS_C_I_12_0125

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

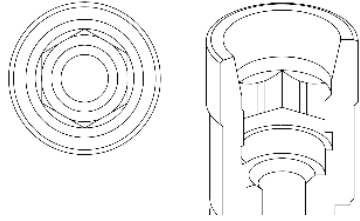

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	2,5 mm			mm			mm			mm			mm		
R	31.322.128.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-	-	-

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Sq. 1.30				
41.320.044.01-2	-	43.618.201.01-2	18	40.320.002.01-2	43.601.102.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0128	LAB SCANBODY	DAS_C_E_0128
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

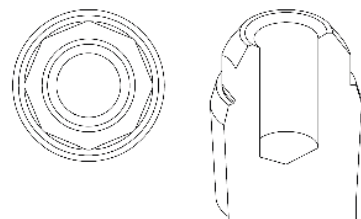

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			mm			mm			mm			mm		
R	31.325.129.01-2	43°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.315.129.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.130.01-2	10	50.315.129.01-2	43.621.410.01-2	34.615.129.01-2	-	-	-	33.390.958.01-2	3	30°
			43.624.410.01-2					33.490.958.01-2	4	
52.412.130.01-2	12	43.630.410.01-2	33.690.958.01-2	6						

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP				
41.320.090.01-2	-	43.618.201.01-2	18	40.320.008.03-2	43.601.108.01-2	-	-	22.615.129.01-2	30.415.007.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0129	LAB SCANBODY	DAS_C_E_0129
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0129	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0129
	DAS_I_12_0129		DAS_C_I_12_0129

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

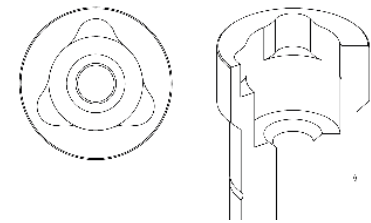

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.322.130.01-2	38°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.130.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	33.345.804.01-2	3	20°
-	-	-	-	-	-	-	-	33.445.804.01-2	4	
-	-	-	-	-	-	-	-	33.645.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.081.01-2	-	43.618.201.01-2	18	40.316.005.08-2	43.601.105.01-2	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0130	LAB SCANBODY	DAS_C_E_0130
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

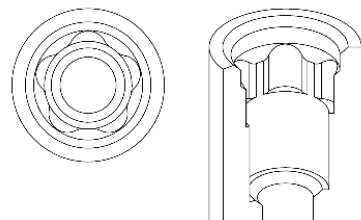

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.323.131.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.131.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	33.345.804.01-2	3	20°
-	-	-	-	-	-	-	-	33.445.804.01-2	4	
-	-	-	-	-	-	-	-	33.645.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.081.01-2	-	43.618.201.01-2	18	40.316.005.08-2	43.601.105.01-2	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0131	LAB SCANBODY	DAS_C_E_0131
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

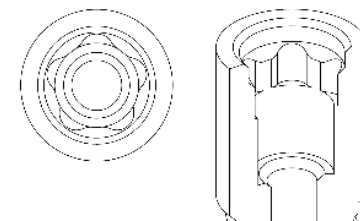

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.324.132.01-2	45°	28°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.132.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
R	-	-	-	-
NR	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	33.345.856.01-2	3	25°
-	-	-	-	-	-	-	-	33.445.856.01-2	4	
-	-	-	-	-	-	-	-	33.645.856.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.316.081.01-2	-	43.618.201.01-2	18	40.316.005.08-2	43.601.105.01-2	-	-	-	30.414.003.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0132	LAB SCANBODY	DAS_C_E_0132
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

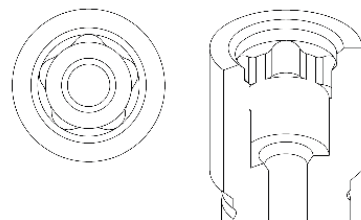

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,7 mm			mm			mm			mm			mm		
R	31.320.136.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.136.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$
		CH=5mm	CH=7mm	CH=9mm
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.128.01-2	10	50.310.136.01-2	43.621.415.01-2	34.610.136.01-2	-	-	-	33.360.754.01-2	3	25°
								33.460.754.01-2	4	
52.412.128.01-2	12							33.660.754.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25				
41.316.071.01-2	-	43.618.201.01-2	18	40.316.004.03-2	43.601.104.01-2	-	-	-	30.410.006.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0136	LAB SCANBODY	DAS_C_E_0136
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0136	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0136
	DAS_I_12_0136		DAS_C_I_12_0136

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

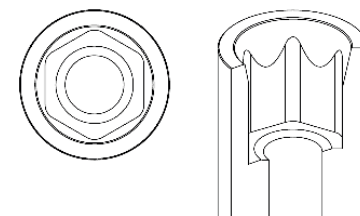

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.324.137.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.137.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$	
-	-	-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-	-	-

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.320.044.01-2	-	43.618.201.01-2	18	40.320.007.04-2	43.601.107.01-2	-	-	-	30.414.008.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0137	LAB SCANBODY	DAS_C_E_0137
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

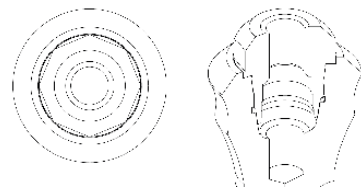

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,5 mm			mm			mm			mm			mm		
R	31.323.149.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.149.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$	
52.410.132.01-2	10	50.313.149.01-2	43.621.410.01-2	34.610.161.01-2	-	-	33.320.704.01-2*	3	25°	
			43.624.410.01-2				33.420.704.01-2*	4		
52.412.132.01-2	12		43.630.410.01-2				33.620.704.01-2*	6		

\*Only for R

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.19				
41.316.079.01-2	-	43.618.201.01-2	18	40.316.014.01-2	-	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0149	LAB SCANBODY	DAS_C_E_0149
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0149	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0149
	DAS_I_12_0149		DAS_C_I_12_0149

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

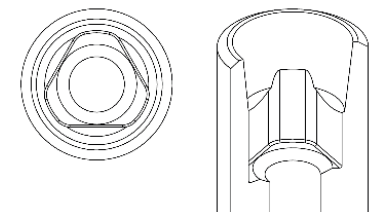



# COMPATIBLE with 0151

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			mm			mm			mm			mm		
R	31.323.151.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
-	-			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.409.123.01-2	9	50.313.151.01-2	43.621.410.01-2 43.624.410.01-2 43.630.410.01-2	34.613.151.01-2	-	-	-	33.390.716.01-2	3	30°
								33.490.716.01-2	4	
								33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER				
41.314.039.01-2	-	43.618.201.01-2 43.624.201.01-2 43.632.201.01-2	18 24 32	-	-	-	-	-	-

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	-	LAB SCANBODY	DAS_C_E_0151
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_9_0151	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_9_0151

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

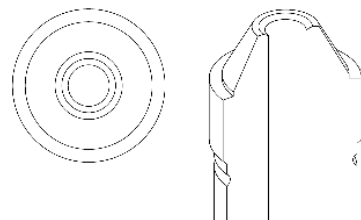

# COMPATIBLE with 0159

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,5 mm			mm			mm			mm			mm		
R	31.320.159.01-2	41°	17°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.159.01-2			-			-			-			-		

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.128.01-2	10	50.310.159.01-2	43.621.415.01-2	34.610.159.01-2	-	-	-	33.335.754.01-2*	3	25°
					33.435.754.01-2*	4				
52.412.128.01-2	12							33.635.754.01-2*	6	

\*Only for R

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER UNIGRIP				
41.314.067.02-2	-	43.618.201.01-2 43.624.201.01-2 43.632.201.01-2	18 24 32	40.314.008.02-2	43.601.108.01-2	22.610.159.01-2	30.410.006.01-2		

## LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0159	LAB SCANBODY	DAS_C_E_0159
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0159 DAS_I_12_0159	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0159 DAS_C_I_12_0159

## LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

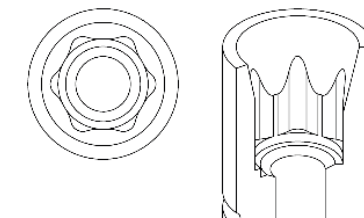

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.320.160.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.160.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.131.01-2	10	50.310.160.01-2	43.621.415.01-2	34.610.160.01-2	-	-	33.315.804.01-2	3	25°
							33.415.804.01-2	4	
52.412.131.01-2	12						33.615.804.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER TORX T6				
41.316.078.01-2	-	43.618.201.01-2	18	40.316.007.01-2	43.601.107.01-2	22.610.160.01-2	30.410.006.01-2		
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0160	LAB SCANBODY	DAS_C_E_0160
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0160	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0160
	DAS_I_12_0160		DAS_C_I_12_0160

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

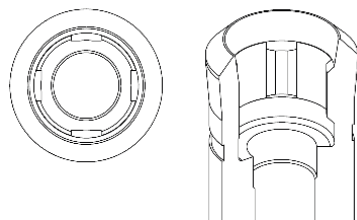

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,5 mm			mm			mm			mm			mm		
R	31.320.161.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.161.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.132.01-2	10	50.310.161.01-2	43.621.415.01-2	34.610.161.01-2	-	-	33.320.704.01-2*	3	25°
							33.420.704.01-2*	4	
52.412.132.01-2	12						33.620.704.01-2*	6	

\*Only for R

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.19				
41.316.079.01-2	-	43.618.201.01-2	18	40.316.014.01-2	-	-	-	30.413.006.01-2	
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0161	LAB SCANBODY	DAS_C_E_0161
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0161	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0161
	DAS_I_12_0161		DAS_C_I_12_0161

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

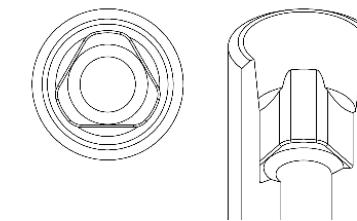

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,5 mm			mm			mm			mm			mm		
R	31.324.162.01-2	45°	24°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.314.162.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.132.01-2	10	50.310.161.01-2	43.621.415.01-2	34.610.161.01-2	-	-	33.320.704.01-2*	3	25°
							33.420.704.01-2*	4	
52.412.132.01-2	12						33.620.704.01-2*	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.19				
41.316.079.01-2	-	43.618.201.01-2	18	40.316.014.01-2	-	-	-	-	30.413.003.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0162	LAB SCANBODY	DAS_C_E_0162
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0162	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0162
	DAS_I_12_0162		DAS_C_I_12_0162

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

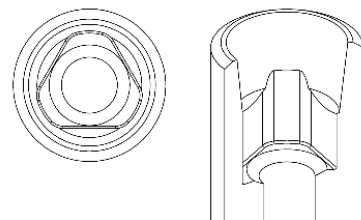

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,5 mm			mm			mm			mm			mm		
R	31.323.163.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.408.112.01-2	8	50.313.163.01-2	43.620.411.01-2	34.613.163.01-2	-	-	33.390.716.01-2	3	30°
							33.490.716.01-2	4	
							33.690.716.01-2	6	

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.19				
41.314.039.01-2	-	43.618.201.01-2	18	40.314.014.01-2	-	-	-	-	30.413.005.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0163	LAB SCANBODY	DAS_C_E_0163
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_8_0163	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_8_0163

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

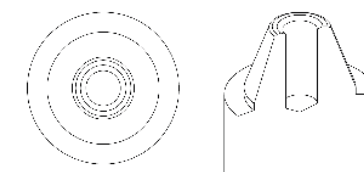

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1 mm			mm			mm			mm			mm		
R	31.320.164.01-2	45°	21°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.164.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.128.01-2	10	50.310.164.01-2	43.621.415.01-2	34.610.164.01-2	-	-	33.345.804.01-2*	3	25°
							33.445.804.01-2*	4	
52.412.128.01-2	12						33.645.804.01-2*	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.312.078.01-2	-	43.618.201.01-2	18	40.312.003.01-2	43.601.103.02-2	-	30.413.006.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0164	LAB SCANBODY	DAS_C_E_0164
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0164	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0164
	DAS_I_12_0164		DAS_C_I_12_0164

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

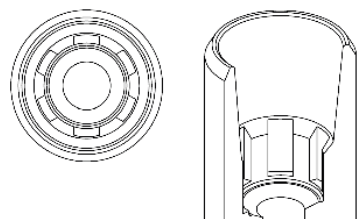

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1 mm			mm			mm			mm			mm		
R	31.323.165.01-2	45°	25°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.313.165.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.132.01-2	10	50.313.165.01-2	43.621.410.01-2	34.613.165.01-2	-	-	33.345.804.01-2*	3	30°
			43.624.410.01-2				33.445.804.01-2*	4	
52.412.132.01-2	12		43.630.410.01-2				33.645.804.01-2*	6	

DYNAMIC SCREWS				STRAIGHT SCREWS			
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.20	ANALOG	LAB SCANBODY
41.314.076.01-2	-	43.618.201.01-2	18	40.314.003.03-2	43.601.103.02-2	-	30.413.002.01-2
		43.624.201.01-2	24				
		43.632.201.01-2	32				

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0165	LAB SCANBODY	DAS_C_E_0165
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_I_10_0165	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	DAS_C_I_10_0165
	DAS_I_12_0165		DAS_C_I_12_0165

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

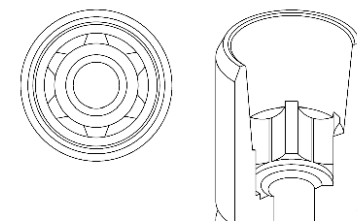

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,9 mm			mm			mm			mm			mm		
R	31.320.166.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.310.166.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-	-

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25				
41.314.084.01-2	-	43.618.201.01-2	18	40.314.004.02-2	43.601.104.01-2	-	-	-	30.410.006.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0166	LAB SCANBODY	DAS_C_E_0166
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

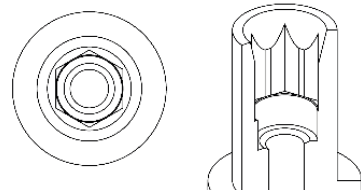

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,9 mm			mm			mm			mm			mm		
R	31.322.167.01-2	43°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.167.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC $\mu$ SCANBODY (LAB/CLIN)				DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL			
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-	-

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.25				
41.316.084.02-2	-	43.618.201.01-2	18	40.316.004.01-2	43.601.104.01-2	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0167	LAB SCANBODY	DAS_C_E_0167
DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-	DYNAMIC $\mu$ SCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

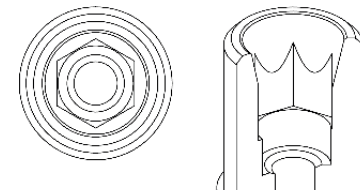



STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,3 mm			mm			mm			mm			mm		
R	31.323.168.01-2	45°	30°	-	-	-	-	-	-	-	-	-	-	-	-
NR	-			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-	-	-

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.314.039.01-2	-	43.618.201.01-2	18	40.314.004.03-2	43.601.104.01-2	-	-	-	30.413.005.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0168	LAB SCANBODY	DAS_C_E_0168
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-
	-		-

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

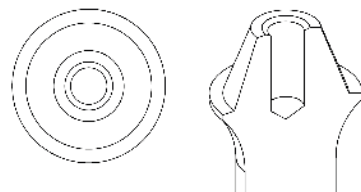

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	0,6 mm			mm			mm			mm			mm		
R	31.322.169.01-2	45°	29°	-	-	-	-	-	-	-	-	-	-	-	-
NR	31.312.169.01-2			-	-	-	-	-	-	-	-	-	-	-	-

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH=7mm	CH=9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED		DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG		COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
52.410.117.01-2	10	50.312.169.01-2	43.621.410.01-2	34.612.169.01-2	-	-	-	33.330.734.01-2	3	25°
			43.624.410.01-2					33.430.734.01-2	4	
52.412.117.01-2	12	43.630.410.01-2	33.630.734.01-2	6						

DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER Hex. 1.27				
41.317.070.01-2	-	43.618.201.01-2	18	40.317.004.02-2	43.601.104.01-2	-	-	-	30.412.001.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES


STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0169	LAB SCANBODY	DAS_C_E_0169
DYNAMIC μSCANBODY (LAB/CLIN)	DAS_I_10_0169	DYNAMIC μSCANBODY (LAB/CLIN)	DAS_C_I_10_0169
	DAS_I_12_0169		DAS_C_I_12_0169

LIBRARY OPTIONS

GH = Gingival Height  
CH = Cement Height

$\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation

R = Rotational / Non-Engaging  
NR = Non Rotational / Engaging

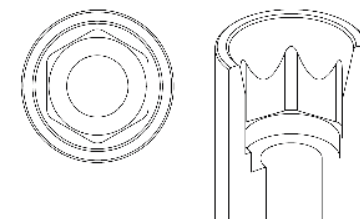

STANDARD DYNAMIC TIBASE®															
	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$	GINGIVAL HEIGHT	$\alpha_s$	$\alpha_c$
	1,2 mm			2,5 mm			3,5 mm			mm			mm		
R	31.323.186.01-2	40°	30°	31.323.186.02-2	20°	18°	31.323.186.03-2	15°	-	-	°	°	-	°	°
NR	31.313.186.01-2			31.313.186.02-2			31.313.186.03-2			-	°	°	-	°	°

DYNAMIC 3TIBASE®				
GINGIVAL HEIGHT	$\alpha_s$	$\alpha_s$	$\alpha_s$	
	CH=5mm	CH= 7mm	CH= 9mm	
-	-	-	-	-
-	-	-	-	-

DYNAMIC μSCANBODY (LAB/CLIN)					DIGITAL ANALOG	DYNAMIC PRE-MILLED	DYNAMIC MILLING TOOL		
SCANBODY	HEIGHT mm	ADAPTOR	SCREWDRIVER ADAPTOR	DIGITAL ANALOG	COBALT-CHROME	$\alpha_{dp}$	DYNAMIC MILLING TOOL	SHANK	$\alpha_{di}$
-	-	-	-	-	-	-	-	-	-
-	-	-	-	-	-	-	-	-	-


DYNAMIC SCREWS				STRAIGHT SCREWS		ANALOG		LAB SCANBODY	
DYNAMIC SCREW	HIGH DYNAMIC SCREW	DYNAMIC SCREWDRIVER	SCREWDRIVER LENGTH (mm)	STRAIGHT SCREW	SCREWDRIVER				
41.316.084.02-2	-	43.618.201.01-2	18	-	-	-	-	-	30.413.002.01-2
		43.624.201.01-2	24						
		43.632.201.01-2	32						

LIBRARY CODES

STANDARD LIBRARY		CAPTIVE SCREW LIBRARY	
LAB SCANBODY	DAS_E_0186	LAB SCANBODY	DAS_C_E_0186
DYNAMIC μSCANBODY (LAB/CLIN)	-	DYNAMIC μSCANBODY (LAB/CLIN)	-

LIBRARY OPTIONS

**GH** = Gingival Height  
**CH** = Cement Height  
 $\alpha_s$  = Standard maximum angulation  
 $\alpha_c$  = Captive maximum angulation  
 $\alpha_{di}$  = Direct to implant maximum angulation  
 $\alpha_{dp}$  = Dynamic Premilled maximum angulation  
**R** = Rotational / Non-Engaging  
**NR** = Non Rotational / Engaging

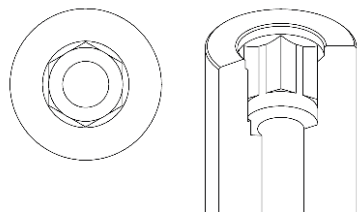



NEW COMPATIBILITIES UNDER DEVELOPMENT

Check new compatibilities under development emailing: [das@dynamicabutment.com](mailto:das@dynamicabutment.com)



# DYNAMIC SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.312.078.01-2	1,2	15 N-cm	7,8	2,65	6	6,55	1,25	2,3	conical	45°	45° Chamfer	HEXALOBULAR 1,70
41.314.039.01-2	1,4	15 N-cm	3,9	1,8	2,1	-	1,8	2,4	straight	-	45° Chamfer	
41.314.040.01-2	1,4	15 N-cm	4	1,85	2	2,78	1,22	2,3	conical	30°	45° Chamfer	
41.314.040.02-2	1,4	15 N-cm	4	1,7	2,25	2,7	1,3	2,3	conical	45°	45° Chamfer	
41.314.043.01-2	1,4	15 N-cm	4,3	1,8	2,03	2,9	1,4	2,3	conical	35°	45° Chamfer	
41.314.045.01-2	1,4	15 N-cm	4,5	2,3	2,5	3,28	1,22	2,3	conical	30°	45° Chamfer	
41.314.052.01-2	1,4	15 N-cm	5,2	2,9	3,4	-	1,8	2,3	straight	-	45° Chamfer	
41.314.064.01-2	1,4	15 N-cm	6,4	2,2	4,21	5,15	1,25	2,3	conical	25°	45° Chamfer	
41.314.064.02-2	1,4	15 N-cm	6,4	2,2	4,65	-	1,75	2,3	straight	-	45° Chamfer	
41.314.067.01-2	1,4	15 N-cm	6,7	2,31	5	5,45	1,25	2,3	conical	45°	45° Chamfer	
41.314.067.02-2	1,4	15 N-cm	6,7	2,5	4,71	5,5	1,2	2,3	conical	35°	45° Chamfer	
41.314.070.01-2	1,4	15 N-cm	7	2,3	5,39	5,65	1,61	2,3	conical	60°	45° Chamfer	
41.314.074.01-2	1,4	15 N-cm	7,4	3,55	5	5,99	1,41	2,3	conical	25°	45° Chamfer	
41.314.076.01-2	1,4	15 N-cm	7,6	2,4	5,9	6,35	1,25	2,3	conical	45°	45° Chamfer	
41.314.084.01-2	1,4	15 N-cm	8,4	2,5	5,92	6,85	1,55	2,3	conical	35°	45° Chamfer	
41.314.105.01-2	1,4	15 N-cm	10,5	2,31	5	5,45	5,05	2,3	conical	45°	45° Chamfer	
41.316.044.01-2	1,6	20 N-cm	4,4	2,5	2,9	-	1,5	2,3	straight	-	Semi-sphere	
41.316.055.01-2	1,6	20 N-cm	5,5	2,4	2,85	4,2	1,3	2,3	conical	23°	45° Chamfer	
41.316.059.01-2	1,6	20 N-cm	5,9	3	4,4	-	1,5	2,3	straight	-	Semi-sphere	
41.316.071.01-2	1,6	20 N-cm	7,1	2,8	5,2	5,53	1,57	2,3	conical	60°	45° Chamfer	
41.316.072.01-2	1,6	20 N-cm	7,2	3,5	5,2	5,85	1,35	2,3	conical	30°	45° Chamfer	
41.316.073.01-2	1,6	20 N-cm	7,3	2,2	4,87	5,56	1,74	2,3	conical	35°	45° Chamfer	
41.316.074.01-2	1,6	20 N-cm	7,4	2,7	5,5	6	1,4	2,3	conical	45°	45° Chamfer	
41.316.076.01-2	1,6	20 N-cm	7,6	3,6	6,1	-	1,5	2,3	straight	-	Semi-sphere	
41.316.078.01-2	1,6	20 N-cm	7,8	2	5,36	7,03	0,81	2,3	conical	15°	45° Chamfer	

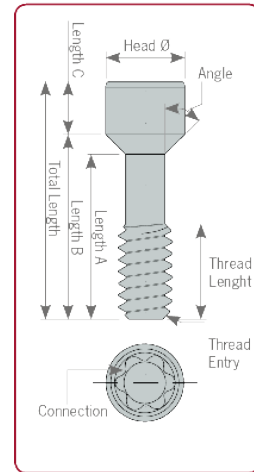
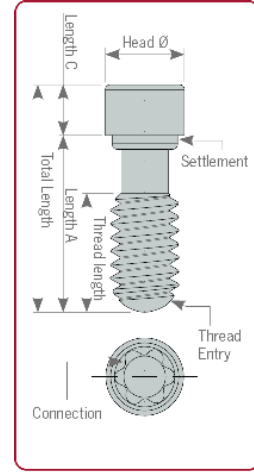


REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.316.079.01-2	1,6	20 N-cm	7,9	2,30	5,42	6,60	1,3	2,3	conical	20°	45° Chamfer	HEXALOBULAR 1,70
41.316.080.01-2	1,6	20 N-cm	8	3,14	6,3	6,51	1,49	2,3	conical	60°	45° Chamfer	
41.316.081.01-2	1,6	20 N-cm	8,1	3	6,35	6,72	1,38	2,3	conical	45°	45° Chamfer	
41.316.084.01-2	1,6	20 N-cm	8,4	3,5	6,8	-	1,6	2,3	straight	-	Semi-sphere	
41.316.084.02-2	1,6	20 N-cm	8,4	2,7	5,85	6,85	1,55	2,3	conical	30°	45° Chamfer	
41.316.094.01-2	1,6	20 N-cm	9,4	2,9	7,65	8	1,4	2,3	conical	45°	45° Chamfer	
41.316.094.02-2	0	20 N-cm	9,4	2,9	7,9	-	1,5	2,3	straight	-	45° Chamfer	
41.316.108.01-2	1,6	20 N-cm	10,803	2,2	4,74	5,56	5,24	2,3	conical	35°	45° Chamfer	
41.316.132.01-2	1,6	20 N-cm	13,2	2,9	7,62	8	5,2	2,3	conical	45°	45° Chamfer	
41.317.065.01-2	N1-72	25 N-cm	6,5	2,4	4,7	5,18	1,33	2,3	conical	45°	45° Chamfer	
41.317.070.01-2	N1-72	25 N-cm	7	2,2	4,96	5,8	1,2	2,3	conical	30°	45° Chamfer	
41.317.071.01-2	N1-72	25 N-cm	7,1	2,6	5,56	5,65	1,45	2,3	conical	70°	45° Chamfer	
41.317.071.02-2	N1-72	25 N-cm	7,1	2,6	5,6	-	1,5	2,3	straight	-	45° Chamfer	
41.317.073.01-2	N1-72	25 N-cm	7,3	2,5	5,5	5,77	1,53	2,3	conical	60°	45° Chamfer	
41.317.106.01-2	N1-72	25 N-cm	10,6	2,6	5,54	5,65	4,95	2,3	conical	70°	Semi-sphere	
41.318.035.01-2	1,8	25 N-cm	3,5	1,9	1,93	2,2	1,4	2,3	conical	60°	45° Chamfer	
41.318.044.01-2	1,8	25 N-cm	4,4	2,75	3	-	1,4	2,3	straight	-	Semi-sphere	
41.318.045.01-2	1,8	25 N-cm	4,5	2,3	2,81	2,9	1,6	2,3	conical	70°	45° Chamfer	
41.318.048.01-2	1,8	25 N-cm	4,8	2,8	3,22	3,65	1,15	2,3	conical	30°	Semi-sphere	
41.318.051.01-2	1,8	25 N-cm	5,1	2,7	3,55	3,7	1,4	2,3	conical	60°	45° Chamfer	
41.318.051.02-2	1,8	25 N-cm	5,1	2,7	3,55	3,7	1,4	2,3	conical	45°	45° Chamfer	
41.318.052.01-2	1,8	25 N-cm	5,2	2,9	3,65	3,8	1,4	2,3	conical	60°	45° Chamfer	
41.318.064.01-2	1,8	25 N-cm	6,4	3,45	4,73	5,1	1,3	2,3	conical	35°	45° Chamfer	
41.318.065.01-2	1,8	25 N-cm	6,5	2,8	5	-	1,5	2,3	straight	-	Semi-sphere	
41.318.066.01-2	1,8	25 N-cm	6,6	4,18	5,05	5,2	1,4	2,3	conical	60°	45° Chamfer	



# DYNAMIC SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.318.067.01-2	1,8	25 N-cm	6,7	2,35	5	5,4	1,3	2,3	conical	45°	45° Chamfer	Hexalobular 1,70
41.318.068.01-2	1,8	25 N-cm	6,8	4	5,25	5,4	1,4	2,3	conical	60°	45° Chamfer	
41.318.071.01-2	1,8	25 N-cm	7,1	2,6	5,56	5,65	1,45	2,3	conical	70°	45° Chamfer	
41.318.074.01-2	1,8	25 N-cm	7,4	3,8	5,8	6,03	1,6	2,3	conical	50°	45° Chamfer	
41.318.075.01-2	1,8	25 N-cm	7,5	3,3	6,1	-	1,4	2,3	straight	-	Semi-sphere	
41.318.076.01-2	1,8	25 N-cm	7,6	2,52	5,8	6,2	1,4	2,3	conical	45°	45° Chamfer	
41.318.077.01-2	1,8	25 N-cm	7,7	2,5	5,81	1,89	1,2	2,3	conical	30°	45° Chamfer	
41.318.080.01-2	1,8	25 N-cm	8	4	6,5	-	1,5	2,3	straight	-	45° Chamfer	
41.318.083.01-2	1,8	25 N-cm	8,3	4,25	6,79	6,95	1,35	2,3	conical	60°	45° Chamfer	
41.320.038.01-2	2	25 N-cm	3,81	1,6	3,25	2,35	1,39	2,35	conical	70°	20° Chamfer	
41.320.044.01-2	2	25 N-cm	4,4	2,45	2,45	3,1	1,3	2,3	conical	45°	45° Chamfer	
41.320.047.01-2	2	25 N-cm	4,7	3	3,3	-	1,4	2,3	straight	-	Semi-sphere	
41.320.048.01-2	2	25 N-cm	4,8	2,7	3,3	3,4	1,4	2,3	conical	60°	45° Chamfer	
41.320.049.01-2	2	25 N-cm	4,9	2,9	3,4	3,5	1,4	2,3	conical	60°	45° Chamfer	
41.320.050.01-2	2	25 N-cm	5	2,8	3,39	3,6	1,4	2,3	conical	30°	Semi-sphere	
41.320.051.01-2	2	25 N-cm	5,1	3,1	3,6	-	1,5	2,3	straight	-	Semi-sphere	
41.320.060.01-2	2	25 N-cm	6	2,7	4,5	-	1,5	2,3	straight	-	Semi-sphere	
41.320.065.01-2	2	25 N-cm	6,5	2,7	5	-	1,5	2,3	straight	-	45° Chamfer	
41.320.066.01-2	2	25 N-cm	6,6	4,18	5,11	5,2	1,4	2,3	conical	60°	45° Chamfer	
41.320.067.01-2	2	25 N-cm	6,7	2,3	3,65	5,68	1,02	2,58	conical	15°	45° Chamfer	
41.320.068.01-2	2	25 N-cm	6,8	4,4	5,3	5,4	1,4	2,3	conical	60°	45° Chamfer	
41.320.070.01-2	2	25 N-cm	7	3	5,6	-	1,4	2,3	straight	-	Semi-sphere	
41.320.074.01-2	2	25 N-cm	7,4	3,3	6	-	1,4	2,3	straight	-	Semi-sphere	
41.320.075.01-2	2	25 N-cm	7,5	2,75	5,93	6,18	1,32	2,3	conical	35°	45° Chamfer	

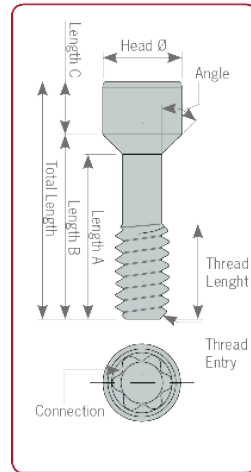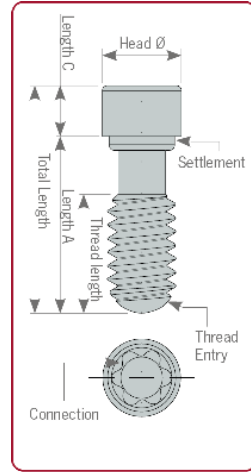

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
41.320.079.01-2	2	25 N-cm	7,9	3,3	6,33	6,5	1,4	2,3	conical	45°	45° Chamfer	Hexalobular 1,70
41.320.082.01-2	2	25 N-cm	8,2	4,7	6,7	-	1,5	2,4	straight	-	Semi-sphere	
41.320.090.01-2	2	25 N-cm	9	4	7,5	-	1,5	2,3	straight	-	Semi-sphere	
41.320.094.01-2	2	25 N-cm	9,4	3	7,85	8	1,4	2,3	conical	45°	45° Chamfer	
41.320.094.02-2	0	25 N-cm	9,4	3	7,9	-	1,5	2,3	straight	-	45° Chamfer	
41.320.117.01-2	2	25 N-cm	11,7	2,75	5,9	6,18	5,52	2,3	conical	35°	Semi-sphere	
41.320.125.01-2	2	25 N-cm	12,5	3,3	6,33	6,5	6	2,3	conical	45°	45° Chamfer	
41.325.054.01-2	2,5	25 N-cm	5,4	3,8	4,1	-	1,3	2,85	straight	-	Semi-sphere	
41.325.067.01-2	2,5	25 N-cm	6,7	4,6	5,1	-	1,6	2,85	straight	-	Semi-sphere	

# DYNAMIC SCREWDRIVER & DYNAMIC SCREWS

## Dynamic Screwdrivers



Screwdriver with hexalobular head, exclusively to the 3.0 Dynamic Abutment® system.

Lengths:  
18, 24, 32mm.

Dynamic Screws are used with the Dynamic TiBase® or milled structures with an angled screw channel. Made of Titanium grade V.





High Dynamic Screw

Dynamic Screw



# STRAIGHT SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
40.312.003.01-2	1,2	15 N-cm	7,85	2,7	6,19	6,55	1,3	1,9	conical	45°	45° Chamfer	Hex. 1,20
40.314.003.01-2	1,4	15 N-cm	3,9	1,91	2,1	-	1,8	2,4	straight	-	45° Chamfer	Hex. 1,20
40.314.003.02-2	1,4	15 N-cm	4	2	2,2	-	1,8	2,3	straight	-	45° Chamfer	Hex. 1,20
40.314.003.03-2	1,4	15 N-cm	7,6	2,4	6,05	6,3	1,3	1,9	conical	45°	45° Chamfer	Hex. 1,20
40.314.003.04-2	1,4	15 N-cm	7,5	2,5	5,45	5,7	1,8	1,85	conical	45°	45° Chamfer	Hex. 1,20
40.314.004.01-2	1,4	15 N-cm	6,3	1,7	4,6	5,1	1,2	2,1	conical	25°	30° Chamfer	Hex. 1,25
40.314.004.02-2	1,4	15 N-cm	8,4	2,5	5,99	6,7	1,7	2	conical	35°	45° Chamfer	Hex. 1,25
40.314.004.03-2	1,4	15 N-cm	4,3	1,8	2,3	-	2	2	straight	-	45° Chamfer	Hex. 1,25
40.314.005.01-2	1,4	15 N-cm	7,6	3,55	5,17	6	1,6	2,15	conical	25°	45° Chamfer	Hex. 1,27
40.314.005.02-2	1,4	15 N-cm	7,5	2,5	5,5	5,7	1,7	2,1	conical	60°	45° Chamfer	Hex. 1,27
40.314.007.01-2	1,4	15 N-cm	4	1,8	2,01	2,8	1,2	2,2	conical	35°	45° Chamfer	Torx T6
40.314.008.01-2	1,4	15 N-cm	3,5	1,8	2,1	-	1,4	2	straight	-	45° Chamfer	Unigrip
40.314.008.02-2	1,4	15 N-cm	6,7	2,5	4,87	5,3	1,4	1,8	conical	35°	45° Chamfer	Unigrip
40.314.012.01-2	1,4	15 N-cm	4,5	1,7	2,01	2,4	2,1	2,15	conical	45°	45° Chamfer	Star 1,50
40.314.014.01-2	1,4	15 N-cm	4,45	2	2,48	-	1,97	2,16	straight	-	45° Chamfer	Hex. 1,19
40.316.002.01-2	1,6	20 N-cm	7	2,79	4,86	5,44	1,56	2,3	conical	45°	45° Chamfer	Sq. 1,30
40.316.002.02-2	1,6	20 N-cm	9,3	3,3	7,3	-	2	2,3	straight	-	Semi-sphere	Sq. 1,30
40.316.003.01-2	1,6	20 N-cm	8,4	2,5	6,6	-	1,8	2	straight	-	45° Chamfer	Hex. 1,20
40.316.003.02-2	1,6	20 N-cm	10,2	2	7,88	8,2	2	2,2	conical	45°	45° Chamfer	Hex. 1,20
40.316.004.01-2	1,6	20 N-cm	8,6	2,7	6,16	6,9	1,7	2	conical	30°	45° Chamfer	Hex. 1,25
40.316.004.02-2	1,6	20 N-cm	8,8	3	6,73	6,8	1,8	2,1	conical	45°	45° Chamfer	Hex. 1,25
40.316.004.03-2	1,6	20 N-cm	6,9	2,2	5,02	5,2	1,7	1,92	conical	60°	45° Chamfer	Hex. 1,25
40.316.005.01-2	1,6	20 N-cm	7,5	3,6	5,33	5,85	1,65	2,15	conical	30°	45° Chamfer	Hex. 1,27
40.316.005.02-2	1,6	20 N-cm	8,2	3,03	6,25	-	2	2,33	straight	-	45° Chamfer	Hex. 1,27
40.316.005.03-2	1,6	20 N-cm	8,25	3,03	6,25	-	2	2,45	straight	-	45° Chamfer	Hex. 1,27
40.316.005.04-2	1,6	20 N-cm	10,5	2,9	8,15	8,4	2,1	2,1	conical	45°	45° Chamfer	Hex. 1,27

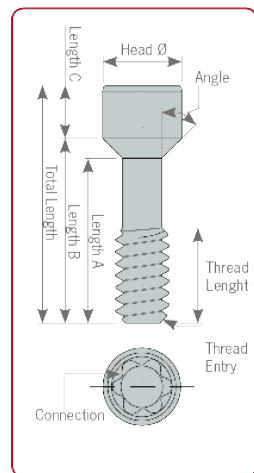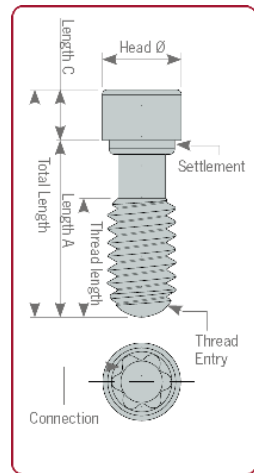



REFERENCE	METRIC	TORQUE	TOTAL LENGTH	THREAD LENGTH	A LENGTH	B LENGTH	C LENGTH	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
40.316.005.06-2	1,6	20 N-cm	3,6	1,8	2,2	-	1,4	2,1	straight	-	45° Chamfer	Hex. 1,27
40.316.005.07-2	1,6	20 N-cm	8,8	2,85	6,73	6,9	1,9	2,15	conical	60	45° Chamfer	Hex. 1,27
40.316.005.08-2	1,6	20 N-cm	9	3,9	0	6,9	2,1	2,18	conical	45°	45° Chamfer	Hex. 1,27
40.316.0 07.01-2	1,6	20 N-cm	7,9	2	5,72	6,9	2,18	2,18	conical	15°	45° Chamfer	Torx T6
40.316.008.01-2	1,6	20 N-cm	7	2,7	5,15	-	1,8	2,3	straight	-	45° Chamfer	Unigrip
40.316.008.02-2	1,6	20 N-cm	7,3	2,7	5,15	5,9	1,4	2,2	conical	35°	45° Chamfer	Unigrip
40.316.012.01-2	1,6	20 N-cm	8	2,65	5,53	6	2	2,15	conical	45°	45° Chamfer	Star 1,50
40.316.014.01-2	1,6	20 N-cm	7,9	2,3	5,42	6,46	1,44	2,2	conical	20°	45° Chamfer	Hex. 1,19
40.317.002.01-2	N1-72	25 N-cm	8,17	3	5,31	5,87	2,3	2,4	conical	45°	45° Chamfer	Sq. 1,30
40.317.004.01-2	N1-72	25 N-cm	7,6	2,8	5,6	5,76	1,84	2,3	conical	70°	45° Chamfer	Hex. 1,27
40.317.004.02-2	N1-72	25 N-cm	7,52	2,2	5,12	5,773	1,75	2,1	conical	30°	45° Chamfer	Hex. 1,25
40.317.005.01-2	N1-72	25 N-cm	7,6	2,5	5,19	5,42	2,18	2,2	conical	60°	45° Chamfer	Hex. 1,27
40.317.005.02-2	N1-72	25 N-cm	7,2	2,4	4,73	5,25	1,95	2,4	conical	45°	45° Chamfer	Hex. 1,27
40.318.002.01-2	1,8	25 N-cm	7	3,2	5,2	-	1,8	2,5	straight	-	45° Chamfer	Sq. 1,30
40.318.002.02-2	1,8	25 N-cm	8,3	2,6	6,6	-	1,7	2,45	straight	-	45° Chamfer	Sq. 1,30
40.318.003.01-2	1,8	25 N-cm	6,8	3,3	5,2	-	1,6	2,3	straight	-	45° Chamfer	Hex. 1,20
40.318.003.02-2	1,8	25 N-cm	8	3,6	6	-	2	2,1	straight	-	45° Chamfer	Hex. 1,20
40.318.004.01-2	1,8	25 N-cm	7,2	4,47	2,3	6,2	1	2,4	conical	30°	45° Chamfer	Hex. 1,25
40.318.004.02-2	1,8	25 N-cm	9,8	5,094	8,3	8,8	1	2,4	conical	30°	45° Chamfer	Hex. 1,25
40.318.004.03-2	1,8	25 N-cm	7,65	3,3	5,17	5,75	1,9	2,4	conical	35°	45° Chamfer	Hex. 1,25
40.318.005.01-2	1,8	25 N-cm	4,5	2,3	2,8	2,9	1,6	2,35	conical	70°	45° Chamfer	Hex. 1,27
40.318.005.02-2	1,8	25 N-cm	7,6	3,8	5,8	6,05	1,55	2,35	conical	50°	45° Chamfer	Hex. 1,27
40.318.006.01-2	1,8	25 N-cm	6	3,18	3,5	3,85	2,15	2,4	conical	45°	45° Chamfer	Hex. 1,50
40.318.007.01-2	1,8	25 N-cm	9,1	4,25	7,22	7,45	1,65	2,18	conical	60°	45° Chamfer	Torx T6
40.318.008.01-2	1,8	25 N-cm	8,3	2,5	6,5	-	1,8	2,45	straight	-	45° Chamfer	Unigrip
40.318.012.01-2	1,8	25 N-cm	7,25	2,4	4,93	5,25	2	2,15	conical	45°	45° Chamfer	Sq. 1,50





# STRAIGHT SCREWS TECHNICAL SPECIFICATIONS

REFERENCE	METRIC	TORQUE	TOTAL LENGHT	THREAD LENGHT	A LENGHT	B LENGHT	C LENGHT	HEAD DIAMETER	SEAT	ANGLE	THREAD ENTRY	CONNECTION
40.318.013.01-2	1,8	25 N-cm	8	2,5	6,01	6,7	1,3	2,2	conical	30°	45° Chamfer	Hex. 1,00
40.320.002.01-2	2	30 N-cm	5	3,06	3,26	3,5	1,5	2,49	conical	45°	45° Chamfer	Cuad. 1,30
40.320.002.02-2	2	30 N-cm	7,45	3	5,7	5,9	1,5	2,4	conical	45°	45° Chamfer	Cuad. 1,30
40.320.002.03-2	2	30 N-cm	10,2	3,15	8,4	-	1,8	2,45	straight	-	45° Chamfer	Cuad. 1,30
40.320.003.01-2	2	30 N-cm	4,7	2,7	3,33	-	1,37	2,35	straight	-	45° Chamfer	Hex. 1,20
40.320.003.02-2	2	30 N-cm	7	3,25	5	-	2	2,4	straight	-	45° Chamfer	Hex. 1,20
40.320.003.03-2	2	30 N-cm	7,9	3,7	5,55	6,05	1,85	2,4	conical	45°	45° Chamfer	Hex. 1,20
40.320.003.04-2	2	30 N-cm	8,4	2,75	5,68	6,35	2,05	2,3	conical	45°	45° Chamfer	Hex. 1,20
40.320.003.05-2	2	30 N-cm	4,8	3,3	3,65	3,9	0,9	2,45	conical	45°	45° Chamfer	Hex. 1,20
40.320.005.01-2	2	30 N-cm	7,6	3,7	6	-	1,6	2,4	straight	-	45° Chamfer	Hex. 1,27
40.320.005.02-2	2	30 N-cm	10,3	4	8,3	-	2	2,45	straight	-	45° Chamfer	Hex. 1,27
40.320.005.03-2	2	30 N-cm	10,3	3,5	8,3	-	2	2,33	straight	-	45° Chamfer	Hex. 1,27
40.320.005.04-2	2	30 N-cm	10,5	3,06	8,15	8,4	2,1	2,5	conical	45°	45° Chamfer	Hex. 1,27
40.320.007.01-2	2	30 N-cm	6,7	2,25	3,59	5,7	1	2,58	conical	15°	45° Chamfer	Torx T6
40.320.007.02-2	2	30 N-cm	7,4	3,3	6	-	1,4	2,3	straight	-	Semi-sphere	Torx T6
40.320.007.03-2	2	30 N-cm	7,6	3	6,1	6,3	1,3	2,4	conical	45°	Semi-sphere	Torx T6
40.320.007.04-2	2	30 N-cm	4,5	2,96	3,21	3,5	1	2,45	conical	45°	45° Chamfer	Torx T6
40.320.008.01-2	2	30 N-cm	7	3,25	5	-	2	2,4	straight	-	45° Chamfer	Unigrip
40.320.008.02-2	2	30 N-cm	7,3	3	5,8	6,2	1,1	2,5	conical	35°	45° Chamfer	Unigrip
40.320.008.03-2	2	30 N-cm	10	3,6	8,5	-	1,5	2,45	straight	-	45° Chamfer	Unigrip
40.325.002.01-2	2,5	30 N-cm	7,41	3,5	4,75	5,29	2,12	2,87	conical	45°	Semi-sphere	Cuad. 1,30
40.325.008.01-2	2,5	30 N-cm	7	2,8	5,6	-	1,4	3,4	straight	-	45° Chamfer	Unigrip

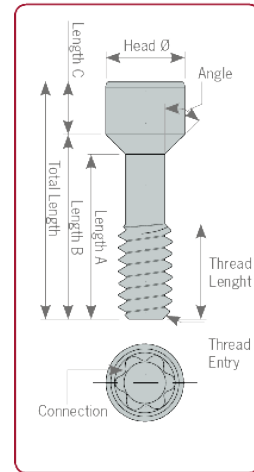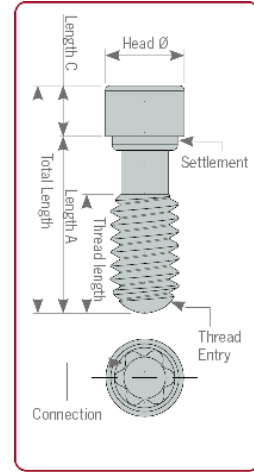

# SCREWDRIVERS & STRAIGHT SCREWS

## Screwdrivers



REF: 43.601.103.02-2  
Hex 1.20mm



REF: 43.601.105.01-2  
Hex. 1.27mm



REF: 43.601.102.01-2  
Squa. 1.30mm



REF: 43.601.108.01-2  
Unigrip



REF: 43.601.104.01-2  
Hex 1.25mm



REF: 43.601.107.01-2  
25mm


Straight screws cover all the thread metrics available on the market. We have several lengths for each metric to make the adaptation to the milled structures easier. Made of Titanium grade V.




Straight Screws

# DYNAMIC SYSTEM SCANBODIES AND COLORS ACCORDING TO COMPATIBILITY

COMPATIBILITY CODE	MAIN COMPATIBILITY	SCANBODY TYPE	ADAPTOR REFERENCE	MIDDLE PIECE	MAGNET SCREW
0002	Biomet 3i Certain RP	HA	52.410.101.01-2		
0007	Astra Evolution 4,2				
0017	MIS C1 RP				
0022	Nobel Biocare Active RP				
0024	Nobel Biocare Branemark RP				N/A
0030	Osstem Implant TS RP				
0040	Zimmer Screw- Vent 3,5				
0057	Biomet 3i Certain WP				
0064	S&M Outlink 4,1				N/A
0005	Astra Lilac			HB	52.410.102.01-2
0018	MIS C1 WP				
0041	Zimmer Screw- Vent 4,5				
0052	Bego S/RI 4,5				
0091	Astra Evolution 4,8				
0001	Biomet 3i Certain NP	HC	52.410.103.01-2		
0004	Astra Aqua				
0021	Nobel Biocare Active NP				
0023	Nobel Biocare Branemark NP				N/A
0029	Osstem Implant TS Mini				
0038	Xive S 3,4				
0083	Klockner Vega RV				

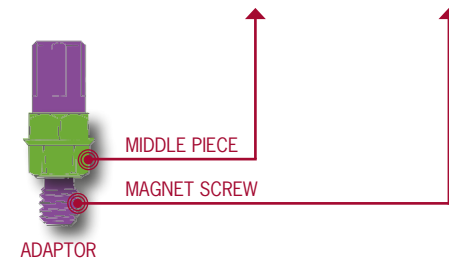


COMPATIBILITY CODE	MAIN COMPATIBILITY	SCANBODY TYPE	REFERENCE	ADAPTOR	MAGNET SCREW
0003	Biomet 3i Osseotite NP	HD	52.410.104.01-2	N/A	
0015	Megagen AnyRidge RP				
0031	S&M Premium Khono 3,3				
0006	Astra Evolution 3,6	HE	52.410.105.01-2		
0019	MIS M4 NP				
0044	Keystone Prima NP				
0075	Ankylos				
0082	Klockner Vega NV				
0008	Astra Evolution Uni Abutment	HF	52.408.113.01-2	N/A	
0009	BTI External Connection NP	HG	52.410.114.01-2	N/A	
0039	Xive S 3,8				
0049	Bego RS/RSX 3	HH	52.410.116.01-2		
0050	Bego S/RI 3,25-3,75	HI	52.410.117.01-2		
0085	Xive S 4,5				
0125	Medentis ICX-Templant 4,1				
0169	Alphabio Conical Standard Connection	HJ	52.410.118.01-2		
0051	Bego S/RI 4,1				
0045	Keystone Prima RP	HK	52.410.120.01-2	N/A	
0058	Biomet 3i Osseotite WP				
0032	S&M Premium Khono 3,80	HL	52.410.121.01-2		
0065	S&M Premium Khono 4,25				

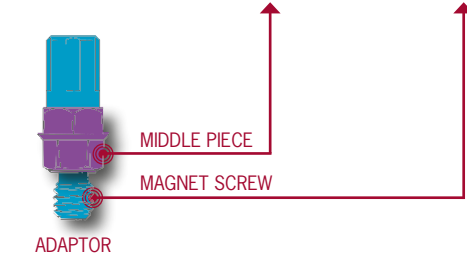


# DYNAMIC SYSTEM SCANBODIES AND COLORS ACCORDING TO COMPATIBILITY

COMPATIBILITY CODE	MAIN COMPATIBILITY	SCANBODY TYPE	REFERENCE	ADAPTOR	MAGNET SCREW
0060	BTI External Connection WP	HM	52.410.122.01-2	N/A	
0047	Neoss ProActive 3,4	HN	52.409.123.01-2		
0048	Neoss ProActive 4,1				
0151	BTI Multi-IM Universal RP			N/A	
0080	Zimmer Screw-Vent 5,7	HO	52.410.124.01-2		
0046	Keystone Prima WP	HP	52.410.125.01-2		
0061	Nobel Biocare Branemark WP			N/A	
0124	Nobel Biocare Active WP				
0081	Bego S/RI 5,50	HR	52.410.126.01-2		
0090	Astra Evolution 3,0	HS	52.410.128.01-2		
0109	Astra Yellow				
0136	Alphabio Conical Hex. Connection				
0159	Nobel Biocare Active 3,0				
0164	Biotech Dental Kontakt 3.0				
0092	Astra Evolution 5,4	HT	52.410.129.01-2		
0025	Nobel Biocare Multi Unit RP	MA	52.410.111.01-2	N/A	
0020	MIS Multi Unit St	MB	52.408.112.01-2	N/A	
0025	Nobel Biocare Multi Unit RP			N/A	
0163	Anthogyr Multi-Unit 4,8			N/A	
0037	Straumann Internal Octagon 4,8	OA	52.410.110.01-2		
0074	Straumann Synocta RP			N/A	
0096	Straumann Internal Octagon 6,5				

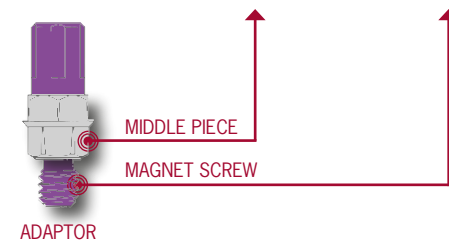


COMPATIBILITY CODE	MAIN COMPATIBILITY	SCANBODY TYPE	REFERENCE	ADAPTOR	MAGNET SCREW
0054	Klockner Essential Cone 4,5	OB	52.410.119.01-2		
0016	MIS C1 NP	SA	52.410.106.01-2		
0033	Straumann Bone Level NP				
0035	Straumann Bone Level RP	SB	52.410.107.01-2		
0010	BTI Internal Connection RP	SC	52.410.115.01-2		
0160	Straumann Tissue Level NNC	SD	52.410.131.01-2		
0011	Camlog Screw-Line 3,8	TA	52.410.108.01-2		
0026	Nobel Biocare Replace NP				
0120	Conelog 3,8				
0012	Camlog Screw-Line 4,3	TB	52.410.109.01-2		
0027	Nobel Biocare Replace RP				
0028	Nobel Biocare Replace WP				
0121	Conelog 4,3	TC	52.410.130.01-2		
0129	Nobel Biocare Replace 6,0				
0149	Anthogyr Axiom REG/PX XNP	TD	52.410.132.01-2		
0162	Anthogyr Axiom REG/PX WP				
0161	Anthogyr Axiom REG/PX RP				
0165	Biotech Dental Kontakt RP				

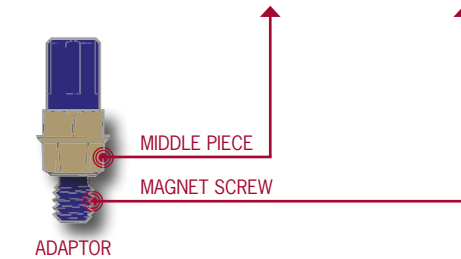

# DYNAMIC MILLING TOOL SPECIFICATIONS

MAIN COMPATIBILITY	REFERENCE	CUTTING DIAMETER	SEAT	CUTTING LENGTH	USEFUL LENGTH (max. drilling depth)	STEM CUTTING DIAMETER	SUPPORT DIAMETER (SHANK)	TOTAL LENGTH
		$\phi_c$		Lc				
ASTRA EVOLUTION 3.0 BEGO RS/RSX 3	33.325.472.01-2	1,4	25	0,4	4,7	0,5	3	50
	33.425.472.01-2	1,4	25	0,4	4,7	0,5	4	50
	33.625.472.01-2	1,4	25	0,4	4,7	0,5	6	50
MEDENTIS ICX TEMPLANT 4.1 STRAUMANN BONE LEVEL NP STRAUMANN BONE LEVEL RP STRAUMANN TISSUE LEVEL NNC	33.315.804.01-2	1,6	15	0,7	8	0,65	3	50
	33.415.804.01-2	1,6	15	0,7	8	0,65	4	50
	33.615.804.01-2	1,6	15	0,7	8	0,65	6	50
ANTHOGRY AXIOM RG/PX XNP ANTHOGRY AXIOM RG/PX RP ANTHOGRY AXIOM RG/PX WP	33.320.704.01-2	1,6	20	0,7	7	0,8	3	50
	33.420.704.01-2	1,6	20	0,7	7	0,8	4	50
	33.620.704.01-2	1,6	20	0,7	7	0,8	6	50
ALPHABIO CONICAL STANDARD CONNECTION ANKYLOS ASTRA EVOLUTION 3.6	33.330.734.01-2	1,6	30	0,7	7,3	0,8	3	50
	33.430.734.01-2	1,6	30	0,7	7,3	0,8	4	50
	33.630.734.01-2	1,6	30	0,7	7,3	0,8	6	50
NOBEL BIOACARE ACTIVE 3.0 NOBEL BIOACARE ACTIVE NP	33.335.754.01-2	1,6	35	0,7	7,5	0,65	3	50
	33.435.754.01-2	1,6	35	0,7	7,5	0,65	4	50
	33.635.754.01-2	1,6	35	0,7	7,5	0,65	6	50
BIOTECH DENTAL KONTACT 3.0 BIOTECH DENTAL KONTACT RP CAMLOG SCREW LINE 3,8/4,3 KLOCKNER VEGA NV OSSTEM IMPLANT TS MINI XIVE S 3,4	33.345.804.01-2	1,6	45	0,7	8	0,65	3	50
	33.445.804.01-2	1,6	45	0,7	8	0,65	4	50
	33.645.804.01-2	1,6	45	0,7	8	0,65	6	50
ALPHABIO CONICAL HEX CONNECTION ASTRA YELLOW CONELOG 3,8/4,3 MIS C1 NP MIS M4 NP	33.360.754.01-2	1,6	60	0,7	7,5	0,65	3	50
	33.460.754.01-2	1,6	60	0,7	7,5	0,65	4	50
	33.660.754.01-2	1,6	60	0,7	7,5	0,65	6	50
ASTRA AQUA BIOMET 3i CERTAIN NP	33.390.754.01-2	1,6	90	0,7	7,5	0,65	3	50
	33.490.754.01-2	1,6	90	0,7	7,5	0,65	4	50
	33.690.754.01-2	1,6	90	0,7	7,5	0,65	6	50
ASTRA EVOLUTION 4.2	33.350.775.01-2	1,7	50	0,7	7,7	0,8	3	50
	33.450.775.01-2	1,7	50	0,7	7,7	0,8	4	50
	33.650.775.01-2	1,7	50	0,7	7,7	0,8	6	50
BIOMET 3i CERTAIN RP/WP MEGAGEN ANYRIDGE RP NOBEL BIOACARE BRANEMARK NP NOBEL BIOACARE REPLACE NP	33.390.805.01-2	1,7	90	0,7	8	0,65	3	50
	33.490.805.01-2	1,7	90	0,7	8	0,65	4	50
	33.690.805.01-2	1,7	90	0,7	8	0,65	6	50

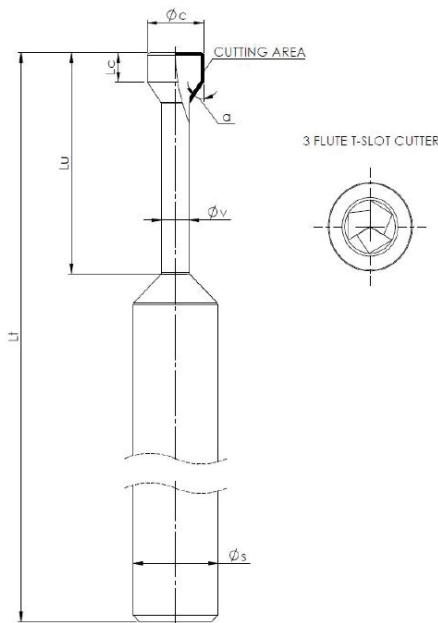

MAIN COMPATIBILITY	REFERENCE	CUTTING DIAMETER	SEAT	CUTTING LENGTH	USEFUL LENGTH (max. drilling depth)	STEM CUTTING DIAMETER	SUPPORT DIAMETER (SHANK)	TOTAL LENGTH
		$\phi_c$		Lc				
BEGO S/RI 3,25-3,75/4,1/4,5/5,50	33.335.676.01-2	1,8	35	1	6,7	0,9	3	50
	33.435.676.01-2	1,8	35	1	6,7	0,9	4	50
	33.635.676.01-2	1,8	35	1	6,7	0,9	6	50
KLOCKNER ESSENTIAL CONE 4.5 KLOCKNER ESSENTIAL CONE 4.5 OCTACONE 12° KLOCKNER ESSENTIAL CONE 4.5 OCTACONE 25° KLOCKNER VEGA RV XIVE S 3,8/4,5	33.345.856.01-2	1,8	45	1	8,5	0,9	3	50
	33.445.856.01-2	1,8	45	1	8,5	0,9	4	50
	33.645.856.01-2	1,8	45	1	8,5	0,9	6	50
MIS C1 RP/WP S&M OUTLINK 3,3/4,1 S&M PREMIUM KHONO 3,3/3,8/4,25	33.360.756.01-2	1,8	60	1	7,5	0,9	3	50
	33.460.756.01-2	1,8	60	1	7,5	0,9	4	50
	33.660.756.01-2	1,8	60	1	7,5	0,9	6	50
ASTRA EVOLUTION UNIT ABUTMENT ZIMMER SCREW-VENT 3.5 ZIMMER SCREW-VENT 4.5 ZIMMER SCREW VENT 5,7	33.370.716.01-2	1,8	70	1	7,1	0,9	3	50
	33.470.716.01-2	1,8	70	1	7,1	0,9	4	50
	33.670.716.01-2	1,8	70	1	7,1	0,9	6	50
ANTHOGRY MULTIHUNT 4.8 BIOMET 3i OSSEOTITE NP/WP BTI EXTERNAL CONNECTION NP/RP/WP BTI MULTIM UNIVERSAL RP KEYSTONE PRIMA NP/RP/WP MIS MULTIHUNT ST NEOSS PROACTIVE 3,4/4,1 NOBEL BIOACARE BRANEMARK RP NOBEL BIOACARE MULTIHUNT RP	33.390.716.01-2	1,8	90	1	7,1	0,9	3	50
	33.490.716.01-2	1,8	90	1	7,1	0,9	4	50
	33.690.716.01-2	1,8	90	1	7,1	0,9	6	50
STRAUMANN INTERNAL OCTAGON 4,8 STRAUMANN INTERNAL OCTAGON 6,5	33.315.708.01-2	2	15	1	7	1	3	50
	33.415.708.01-2	2	15	1	7	1	4	50
	33.615.708.01-2	2	15	1	7	1	6	50
STRAUMANN SYNOCTA RP	33.330.708.01-2	2	30	1	7	1	3	50
	33.430.708.01-2	2	30	1	7	1	4	50
	33.630.708.01-2	2	30	1	7	1	6	50
NOBEL BIOACARE ACTIVE RP NOBEL BIOACARE ACTIVE WP	33.335.758.01-2	2	35	1	7,5	1	3	50
	33.435.758.01-2	2	35	1	7,5	1	4	50
OSSTEM IMPLANT TS RP	33.335.758.01-2	2	35	1	7,5	1	6	50
	33.635.758.01-2	2	35	1	7,5	1	6	50
ASTRA EVOLUTION 4.8/5.4 ASTRA LILAC NOBEL BIOACARE BRANEMARK WP NOBEL BIOACARE REPLACE RP/WP/6.0	33.345.808.01-2	2	45	1	8	1	3	50
	33.445.808.01-2	2	45	1	8	1	4	50
	33.645.808.01-2	2	45	1	8	1	6	50
ASTRA EVOLUTION 4.8/5.4 ASTRA LILAC NOBEL BIOACARE BRANEMARK WP NOBEL BIOACARE REPLACE RP/WP/6.0	33.390.958.01-2	2	90	1	9,5	1	3	50
	33.490.958.01-2	2	90	1	9,5	1	4	50
	33.690.958.01-2	2	90	1	9,5	1	6	50

Reference code:

33.445.804.01-2  
 Cutting seat: 33  
 Cutting diameter code: 445  
 Shank: 804  
 Useful length: 01  
 Total length: 2



**DMTONE**  
DYNAMIC MILLING TOOL

# SCREWDRIVER ADAPTOR

## Screwdriver for the Dynamic µScanbody System

Ref. 43.621.410.01-2  
Screwdriver with manual handle  
Standard length: 21mm



Ref. 43.624.410.01-2  
Contra-angle  
Length: 24mm




Ref. 43.630.410.01-2  
Contra-angle  
Length: 30mm



Ref. 43.621.415.01-2  
Tiny  
Screwdriver with manual handle  
Length: 21mm



Ref. 43.620.411.01-2  
Multi Unit  
Contra-angle  
Length: 20 mm



# COMPLEMENTS

## Manual handle

Made of stainless steel.  
They are used to connect screwdriver bits with the contra-angle connection



**Large manual handle for laboratory** Ref. 49.601.000.03-2  
Ideal to manipulate models in the laboratory.  
Length: 55.65mm.



**Manual handle for clinic** Ref. 49.601.000.01-2  
Clinic handle: used to position the prosthesis in the mouth prior to torque control in the clinic.  
Length: 15.65mm.

## Manual torque wrench adapter prosthetic

Piece to connect the screwdriver with contra-angle connection to the torque wrench.



Universal Manual torque wrench adapter  
Ref. 49.604.000.05-2  
4mm Square connection



Straumann Manual torque wrench adapter  
Ref. 49.604.000.07-2  
Straumann connection



Nobel Biocare Manual torque wrench adapter  
Ref. 49.604.000.08-2



## Universal manual torque wrench prosthetic

Ref. 11.990.990.07-2  
Torque wrench.  
4mm square connection.  
Torque 10-35N.c

# IDENTIFICATION PRODUCT

The label accompanying all Dynamic Abutment® Solutions products contains all the information the user requires. The product label contains detailed information of the contents of the blister pack. The symbols found on the identity labels correspond to the international product identification standards. All products are supplied with their corresponding instructions for use which include an explanation of each of the symbols found on the product label.

Identification of compliance with the requirements of applicable EC legislation

Manufactured

Batch Number

Product reference

Material

Content information

Extended information

Non-reusable

Refer to the instructions for use

Do not use is packaging is damaged

Non sterile product

Labels include: REF 31.312.040.02-2, LOT 04753T18-1, MAT TITANIO, ES Interfase Dinamica no rotatoria G1.5 Comp.0040, EN Engaging Dynamic Ti-Base G1.5 Comp.0040, Talladum España, S.L., Av. Blondel, Ed. planta 3ª 08002 LLEIDA - Spain, +34 973 289 580, www.dynamicabutment.com

# SECURITY & TRACEABILITY

All of our products are patented and manufactured under very strict quality guidelines. With the 3.0 Dynamic System, we provide a card for the laboratory and the clinic to identify the position in Dynamic System is located. We exercise complete control over the traceability of our products to fulfil the current health legislation. This helps repositioning the material and inform about the importance of using the appropriate tools when handling the Dynamic System components.

Dynamic Abutment Solutions

SPAIN: +34 973 289 580, span@dynamicabutment.com, www.dynamicabutment.es

INTERNATIONAL: +34 973 459 709, ds@dynamicabutment.com, www.dynamicabutment.com

Fabricado por / Manufactured by: Talladum España SL

3.0 Sistema Dinámico Location Dynamic System

17 18 19 20 21 22 23 24 25 26 27

27 28 29 30 31 32 33 34 35 36 37

REF: /

LOTE/BATCH: /

3.0 Ejemplar Laboratorio Laboratory Exemplar

3.0 Ejemplar Clínica Clinic Exemplar

Completar la información y adjuntar en la ficha del paciente. Complete information and enclose it to the patient file.

Paciente / Patient Name: /

Ref: / Lote / Batch: /

Fecha / Date: /

Localización Sistema Dinámico Location Dynamic System

17 18 19 20 21 22 23 24 25 26 27

27 28 29 30 31 32 33 34 35 36 37

Recomendación / Advice: Realizar torque de laboratorio para la instalación de la prótesis. Use laboratory torque when assembling prosthesis.

Recomendación / Advice: Para la posición definitiva de la prótesis, usar los torques de ajuste. Colocar en los torques de ajuste de cada sistema / 3.0 miembro con un torque de ajuste. Para la posición definitiva de la prótesis, usar los torques de ajuste.



# TALLADIUM GUARANTEE

## TERMS AND CONDITIONS

These guarantee terms and conditions ("T&C") cover the entire range of Talladium products ("Products"), manufactured by TALLADIUM ESPAÑA S.L. and distributed by Geoda Medical S.L. or official dealers. The guarantee described in these T&C is exclusively in benefit of the clinician ("Clinician") and of the dental technician ("Technician") and not for the benefit of third parties or institutions, including patients.

## GUARANTEE PERIOD

TALLADIUM ESPAÑA S.L. offers a lifelong guarantee for its entire range of products starting from the date of issue of the invoice.

## GUARANTEE SCOPE

Subject to the limitations and exceptions described in these T&C, TALLADIUM ESPAÑA S.L. will offer the following benefits:

**QUALITY:** If there are defects in the materials or in the manufacturing of the Product, TALLADIUM ESPAÑA S.L. will replace the Product with no additional cost.

**SAFETY:** If, having complied with all the product indications, the prosthesis should have to be made again, due to a fault in the Dynamic Abutment® or Dynamic Titanium Base® system, TALLADIUM ESPAÑA S.L. will replace the abutments and screws necessary to remake the prosthesis, as well as the costs derived from its manufacturing.

In case of having used our products and having complied with all the product indications, the implants suffer any damage, TALLADIUM ESPAÑA S.L. will pay the cost of the implants. This coverage will only be valid during the first 6 months after the collocation of the prosthesis which includes our products.

## CLAIM REQUIREMENTS AND PROCEDURE

To receive the benefits indicated in these T&C, the treating Clinician must satisfy the following requirements:

- The claim must be notified to TALLADIUM ESPAÑA S.L. within (30) days since the date the claimed defect was detected.
- This requires that the Clinician or Technician must contact the customer service department by telephone or by e-mail to make the claim.
- A claim form will be completed, which, together with a document or report which justifies the faulty Product and the faulty Product itself, will be sent by the customer to TALLADIUM ESPAÑA S.L. offices, within the previously indicated period.
- Clinicians or Technicians presenting a claim in agreement with these T&C must be up to date in any payments owing to TALLADIUM ESPAÑA S.L. or to any of its subsidiaries, at the time when the claim form is presented.
- All the use procedures of our Products must be carried out in agreement with the instructions of TALLADIUM ESPAÑA S.L. as well as in accordance with commonly accepted dentistry practices.
- The expenses derived from this procedure will be assumed by the customer. The return shipping costs will be assumed by TALLADIUM ESPAÑA S.L. in all those cases covered by these T&C.

Regardless of the guarantee rights, claims should be notified as soon as possible in order to comply with regulatory requirements.

## GENERAL LIMITATIONS OF THIS GUARANTEE

With the exception of the guarantee described in these T&C, neither TALLADIUM ESPAÑA S.L. nor its representatives, nor third parties manufacturing or distributing the Products, represent or offer a guarantee, agreement or any other express or implicit, oral or written, commitment, with respect to the Products (without limitation), including guarantees involved in the marketing, durability or suitability for individual uses or purposes.

In addition and within the maximum extent permitted by the relative law, TALLADIUM ESPAÑA S.L. rejects (on its own behalf, and on behalf of its representatives and third parties that manufacture or distribute Products) any responsibility with respect to any direct or indirect damage caused, which may result from or be a consequence of the design, composition of the dental prosthesis into which the Products are integrated.

## GUARANTEE EXCLUSIONS

TALLADIUM ESPAÑA S.L. limits this guarantee to:

- Transformed abutments that form part of the dental prosthesis. But not the screws used to anchor them.
- Clinical screws that have been in the mouth for more than 2 years.

## AMENDMENT OR SUSPENSION OF THE GUARANTEE

TALLADIUM ESPAÑA S.L. reserves the right to amend or withdraw these T&C at any time and without prior notification. Any modification or suspension shall not affect products already placed in patients.

Ed.2019-01



AV. BLONDEL, 54 3º · 25002 · LLEIDA (SPAIN)  
TEL. +34 873 450 709  
das@dynamicabutment.com  
www.dynamicabutment.com





AV. BLONDEL, 54 3º · 25002 · LLEIDA (SPAIN)  
TEL. +34 873 450 709  
das@dynamicabutment.com  
www.dynamicabutment.com

DYNAMIC ABUTMENT® SOLUTIONS